


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV033019\
 Data File : VV010015.D
 Acq On : 30 Mar 2019 12:06
 Operator : SY/MD
 Sample : BFB80
 Misc : 5.00G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB80

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Title : VOC Analysis
 Last Update : Tue Apr 02 08:12:49 2019

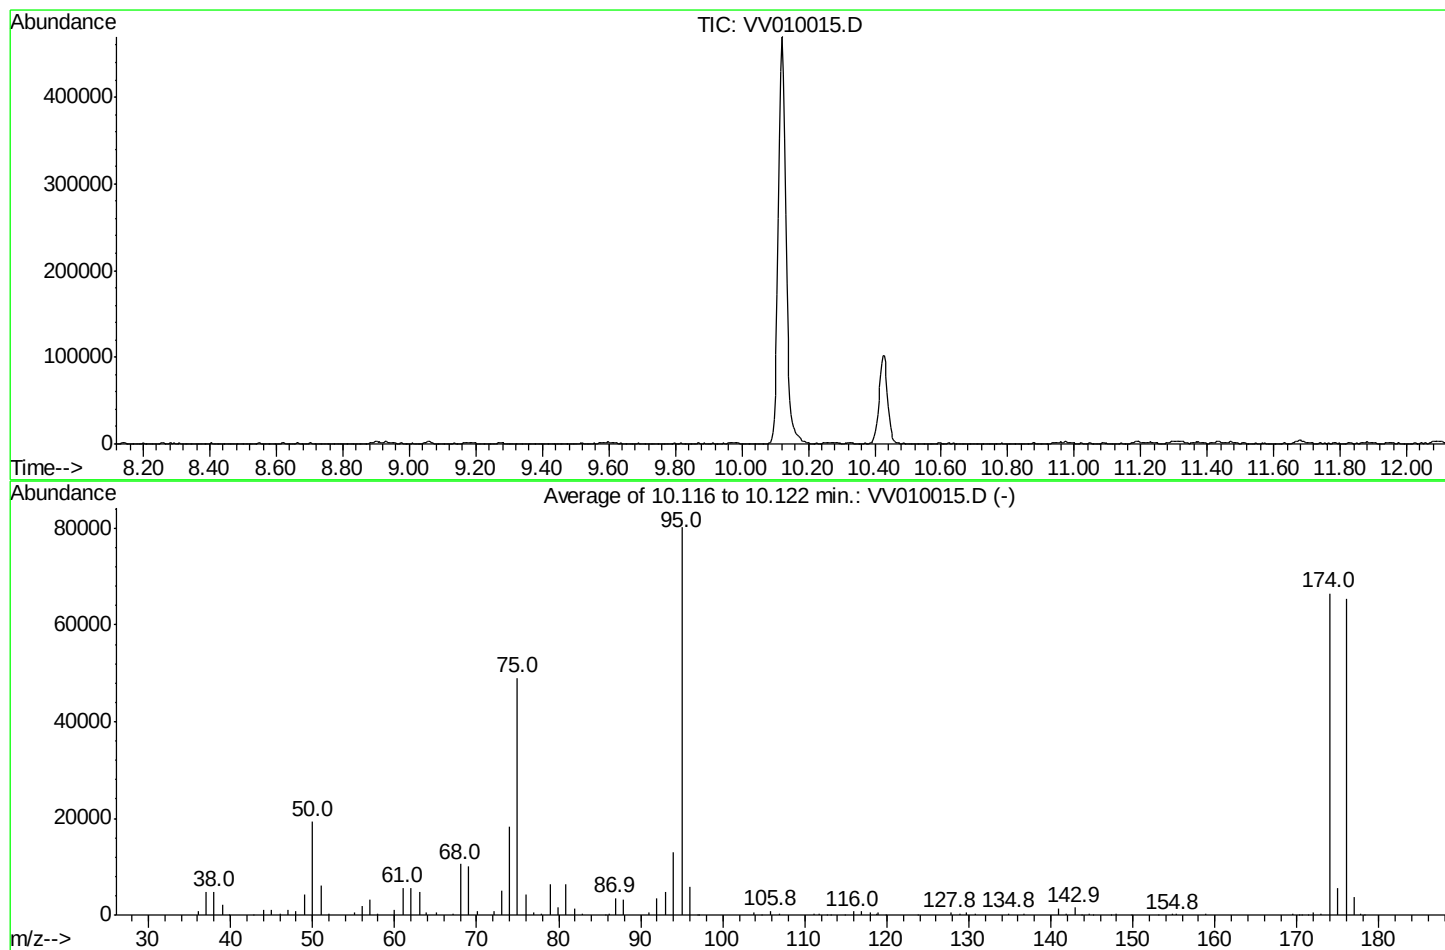

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	19229	PASS
75	95	30	80	61.2	49058	PASS
95	95	100	100	100.0	80205	PASS
96	95	5	9	7.3	5876	PASS
173	174	0.00	2	0.6	400	PASS
174	95	50	120	83.0	66533	PASS
175	174	5	9	8.4	5589	PASS
176	174	95	101	98.4	65437	PASS
177	176	5	9	5.8	3767	PASS

Scan 2795 (10.077 min): VV010015.D
BFB80

m/z	Abundance
37.20	147.0
39.90	120.0
44.10	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.10	843.0
37.00	4633.0
38.00	4653.0
39.00	2060.0
39.90	158.0
44.00	1127.0
45.00	952.0
46.10	192.0
47.00	1016.0
47.90	881.0
49.10	3883.0
50.00	18808.0
51.00	5786.0
52.00	185.0
55.10	431.0
56.00	1710.0
57.00	2859.0
57.90	320.0
59.90	1184.0
61.00	5590.0
62.00	5292.0
63.00	4553.0
63.90	485.0
65.10	558.0
67.20	243.0
68.00	9967.0
69.00	9506.0
70.10	956.0
72.10	595.0
73.00	5034.0
74.00	17040.0
75.00	46952.0
76.00	4112.0
76.90	418.0
77.90	348.0
78.90	6223.0
79.90	1483.0
80.90	5654.0
81.90	1316.0
82.90	181.0
85.70	153.0
86.10	140.0
86.90	3253.0
87.90	2842.0
91.00	536.0
92.00	3385.0
93.00	4530.0
94.00	12593.0
95.00	76328.0
96.00	5411.0
96.90	187.0
103.80	398.0
104.80	118.0
105.80	830.0
106.90	181.0
111.00	172.0
111.80	130.0
113.10	140.0
114.90	109.0
115.90	666.0
116.90	775.0
117.90	537.0
118.80	530.0
119.90	129.0
127.80	376.0
129.00	126.0
129.70	512.0
130.80	250.0
134.90	290.0
136.80	213.0
140.90	1242.0
142.00	190.0
142.90	1610.0
144.80	217.0
147.90	213.0
149.70	138.0
154.80	209.0
155.20	176.0
158.90	175.0
169.50	143.0
172.00	623.0
174.00	60896.0
175.00	5338.0
176.00	60336.0
177.00	3599.0
177.80	154.0
178.20	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.10	963.0
37.00	4996.0
38.00	5015.0
39.00	2185.0
39.90	150.0
42.80	110.0
44.00	1284.0
45.00	1142.0
46.10	190.0
47.00	1156.0
47.90	893.0
49.10	4344.0
50.00	19904.0
51.00	6429.0
52.00	165.0
55.10	443.0
56.00	1958.0
57.00	3379.0
57.90	337.0
59.90	1222.0
61.00	5764.0
62.00	5591.0
63.00	4865.0
63.90	556.0
65.00	519.0
67.20	326.0
68.00	10770.0
69.00	10222.0
70.10	889.0
72.10	719.0
73.00	5215.0
74.00	18792.0
75.00	50208.0
76.00	4216.0
77.00	444.0
77.90	344.0
79.00	6466.0
79.90	1599.0
80.90	6420.0
81.90	1468.0
82.90	275.0
85.80	131.0
86.10	149.0
86.90	3670.0
87.90	3274.0
91.10	548.0
92.00	3556.0
93.00	4858.0
94.00	13268.0
95.00	82816.0
96.00	6164.0
97.10	167.0
103.80	468.0
104.80	142.0
105.90	837.0
106.90	186.0
111.10	230.0
111.80	164.0
112.80	169.0
114.80	139.0
116.00	787.0
116.90	726.0
118.00	675.0
119.00	597.0
119.90	127.0
123.70	134.0
127.80	448.0
128.90	148.0
129.70	425.0
130.80	203.0
134.80	295.0
136.80	212.0
140.90	1395.0
141.90	205.0
142.90	1550.0
143.70	124.0
144.70	220.0
147.30	102.0
147.90	228.0
149.80	153.0
154.80	257.0
155.30	187.0
158.80	189.0
169.50	161.0
170.20	106.0
170.60	145.0
171.90	599.0
174.00	68512.0
175.00	5672.0
176.00	67808.0
177.00	3834.0
177.80	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

178.20

146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.10	948.0
37.00	5110.0
38.00	4882.0
39.00	2075.0
40.00	128.0
42.80	144.0
44.00	1282.0
45.00	1184.0
46.10	135.0
47.00	1153.0
47.90	724.0
49.10	4351.0
50.00	18976.0
51.00	6432.0
52.00	128.0
55.00	450.0
56.00	2008.0
57.00	3650.0
57.90	268.0
60.00	1107.0
61.00	5445.0
62.00	5528.0
63.00	4765.0
63.90	515.0
65.00	442.0
67.10	322.0
68.00	10737.0
69.00	10331.0
70.00	904.0
72.10	724.0
73.00	4883.0
74.00	19296.0
75.00	50016.0
76.00	4246.0
77.00	440.0
77.90	320.0
79.00	6117.0
79.90	1533.0
80.90	6661.0
81.90	1500.0
82.90	314.0
86.10	227.0
86.90	3560.0
87.90	3338.0
91.10	455.0
91.90	3059.0
93.00	4717.0
94.00	12993.0
95.00	81472.0
96.00	6054.0
97.10	203.0
103.90	604.0
105.90	734.0
106.90	181.0
111.10	246.0
111.80	164.0
112.70	213.0
114.80	138.0
116.00	770.0
116.80	677.0
118.00	735.0
119.00	756.0
123.70	182.0
127.80	596.0
128.90	178.0
129.80	339.0
130.90	183.0
134.80	256.0
136.70	193.0
140.90	1321.0
141.80	214.0
142.90	1584.0
143.70	109.0
144.60	197.0
145.10	221.0
147.30	106.0
147.90	232.0
149.80	136.0
153.10	109.0
154.90	211.0
155.30	126.0
158.80	156.0
169.50	139.0
170.20	117.0
170.60	173.0
171.30	322.0
172.00	565.0
172.90	1202.0
174.00	70192.0
175.00	5757.0
176.00	68168.0
177.00	3870.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

177.80

209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80