
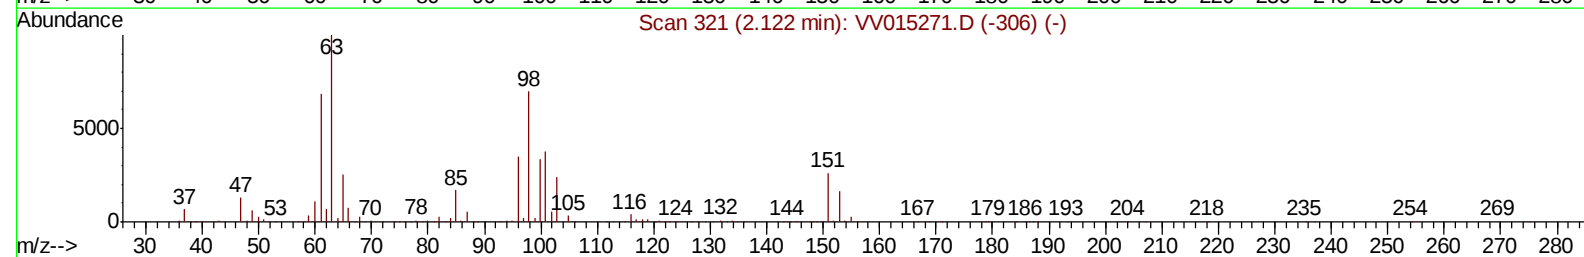
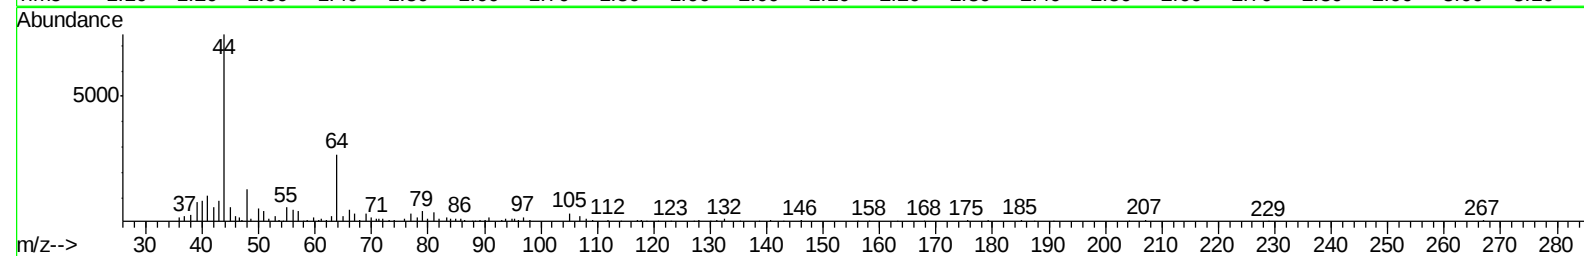


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015289.D
 Acq On : 30 Mar 2020 22:08
 Operator : SY/MD
 Sample : L1976-11DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 02:22:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 02:12:40 2020
 Response via : Initial Calibration

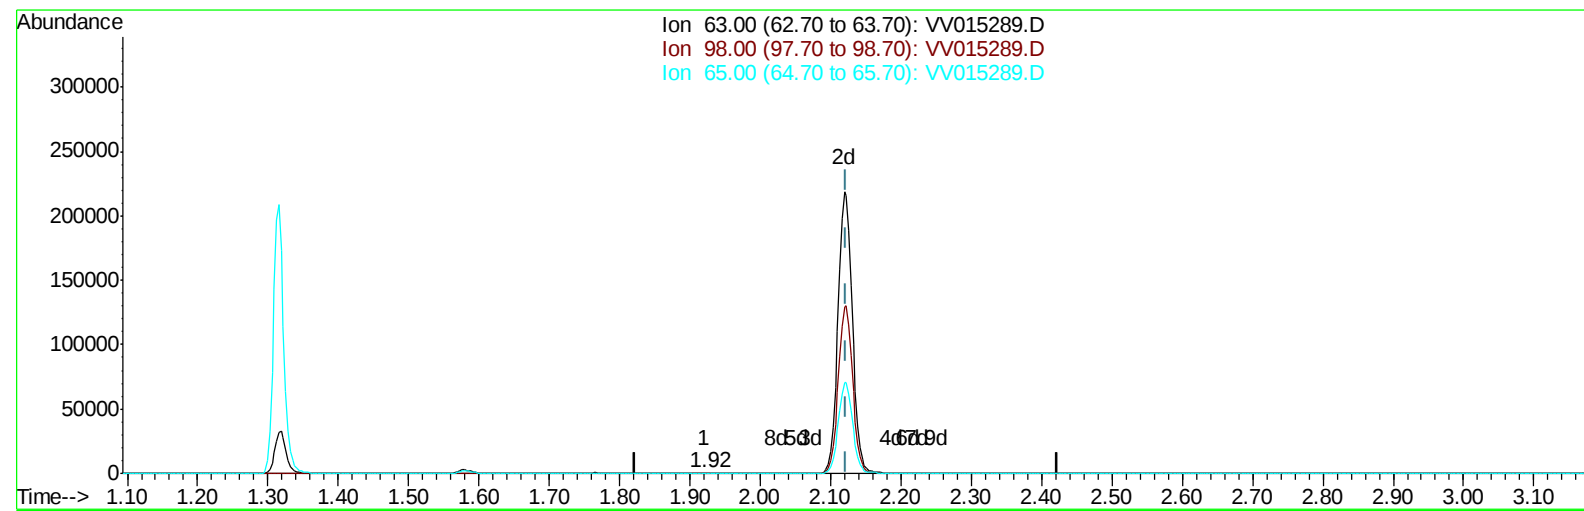

TIC: VV015289.D

(11) 1,1-Dichloroethene-d2 (S)

1.920min (-0.202) 0.03ug/L

response 321

Ion	Exp%	Act%
63.00	100	100
98.00	72.00	64.17
65.00	23.00	16.20
0.00	0.00	0.00