

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015283.D
 Acq On : 30 Mar 2020 19:43
 Operator : SY/MD
 Sample : L1975-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH5

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:22:16 PM

Quant Time: Mar 31 02:21:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 02:12:40 2020
 Response via : Initial Calibration

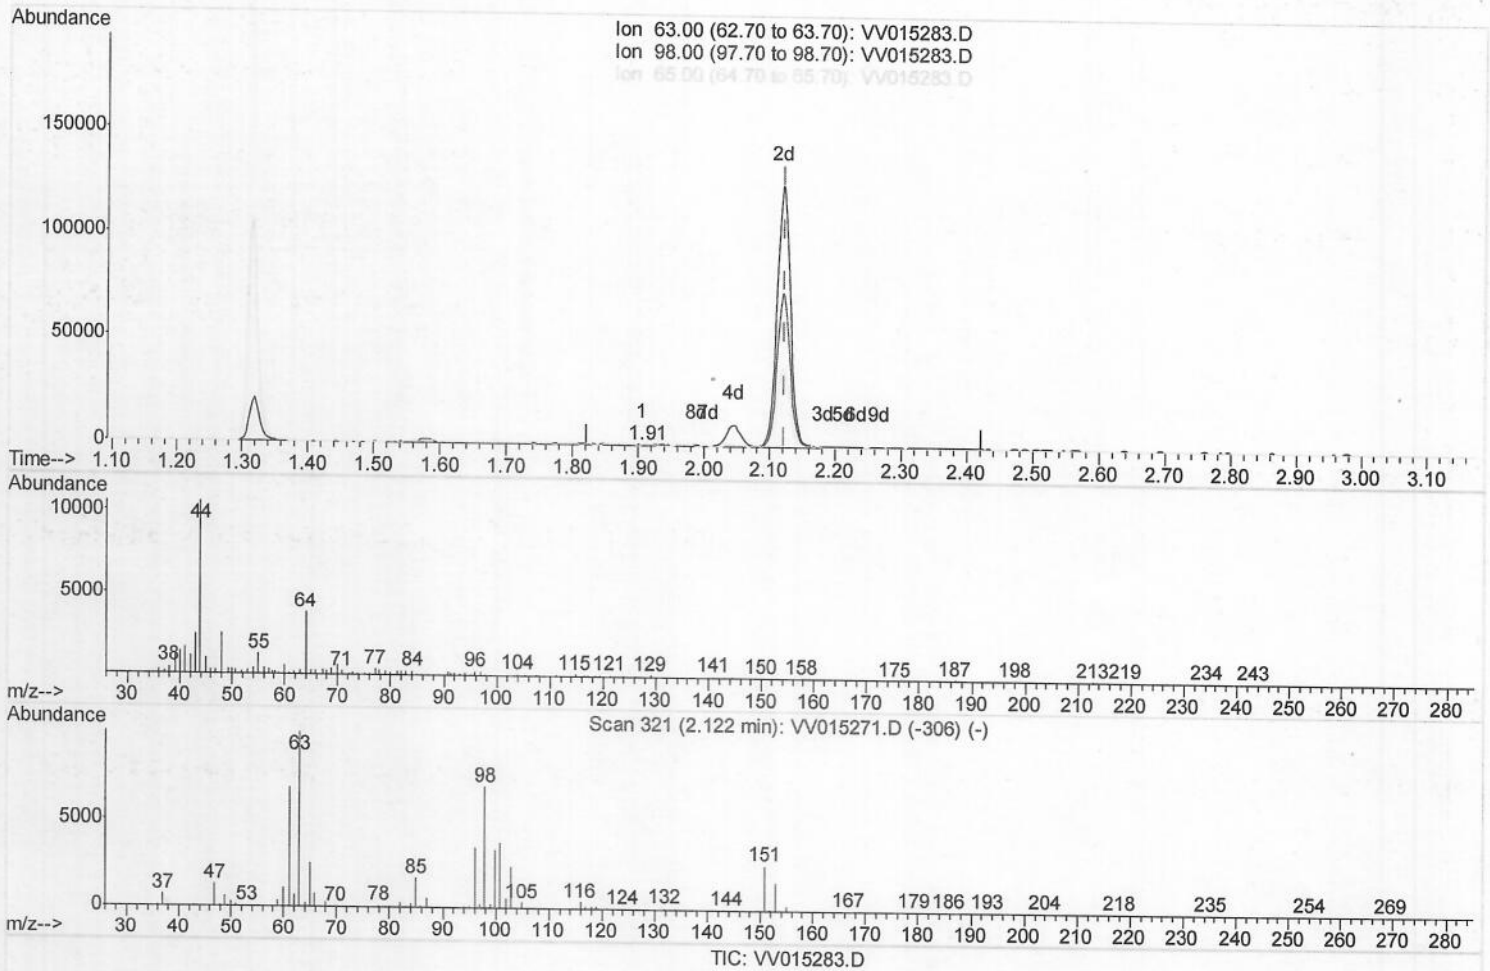

(11) 1,1-Dichloroethene-d2 (S)

1.907min (-0.215) 0.04ug/L

response 365

Ion	Exp%	Act%
63.00	100	100
98.00	72.00	60.55
65.00	23.00	26.03
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015283.D
 Acq On : 30 Mar 2020 19:43
 Operator : SY/MD
 Sample : L1975-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH5

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:22:16 PM

Quant Time: Mar 31 02:21:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 02:12:40 2020
 Response via : Initial Calibration

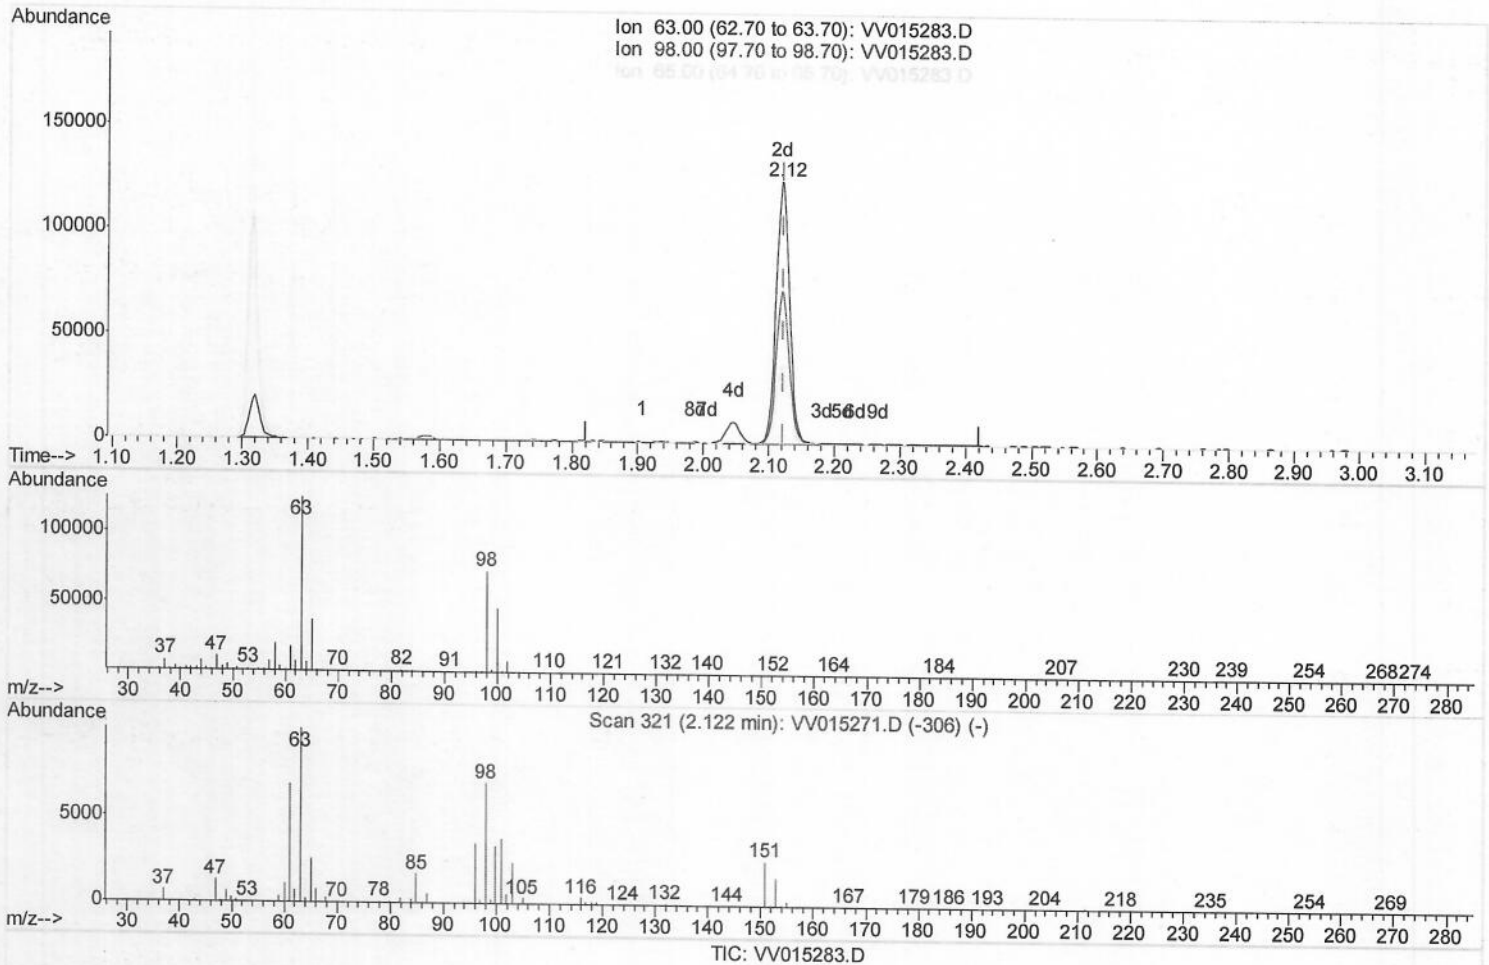

(11) 1,1-Dichloroethene-d2 (S)

2.119min (-0.003) 19.31ug/L m

response 179544

Ion	Exp%	Act%
63.00	100	100
98.00	72.00	0.12#
65.00	23.00	0.05#
0.00	0.00	0.00

MD
 04/2/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015283.D
 Acq On : 30 Mar 2020 19:43
 Operator : SY/MD
 Sample : L1975-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH5

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:22:16 PM

Quant Time: Mar 31 05:03:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 02:12:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	591420	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	570147	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	254405	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	110516	25.63	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	51.26%#		
7) Chloroethane-d5	1.58	69	119841	29.86	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	59.72%#		
11) 1,1-Dichloroethene-d2	2.12	63	179544m	19.31	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	38.62%#		
21) 2-Butanone-d5	3.93	46	257482	91.30	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.30%		
24) Chloroform-d	4.38	84	264984	34.18	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	68.36%#		
26) 1,2-Dichloroethane-d4	5.06	65	177836	35.10	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	70.20%		
32) Benzene-d6	5.08	84	475743	31.96	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	63.92%#		
36) 1,2-Dichloropropane-d6	6.09	67	163091	35.04	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	70.08%		
41) Toluene-d8	7.34	98	436632	30.32	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	60.64%#		
43) trans-1,3-Dichloropropene-	7.64	79	72346	28.54	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	57.08%#		
47) 2-Hexanone-d5	8.11	63	222423	101.87	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.87%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	265378	38.63	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	77.26%		
64) 1,2-Dichlorobenzene-d4	11.65	152	178477	35.25	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	70.50%#		

MD
 04/2/2020

Target Compounds

					Ovalue
5) Vinyl chloride	1.32	62	299396	60.061	ug/L 99
13) Acetone	2.21	43	45926	23.865	ug/L 81
19) 1,1-Dichloroethane	3.22	63	6469	0.947	ug/L 93
20) cis-1,2-Dichloroethene	3.95	96	7449	1.808	ug/L # 92
22) 2-Butanone	4.01	43	106910	38.110	ug/L 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015283.D
 Acq On : 30 Mar 2020 19:43
 Operator : SY/MD
 Sample : L1975-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH5

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:22:16 PM

Quant Time: Mar 31 05:03:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 02:12:40 2020
 Response via : Initial Calibration

