

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015298.D
 Acq On : 31 Mar 2020 02:36
 Operator : SY/MD
 Sample : L1975-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:21:17 PM

Quant Time: Mar 31 06:28:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 06:20:52 2020
 Response via : Initial Calibration

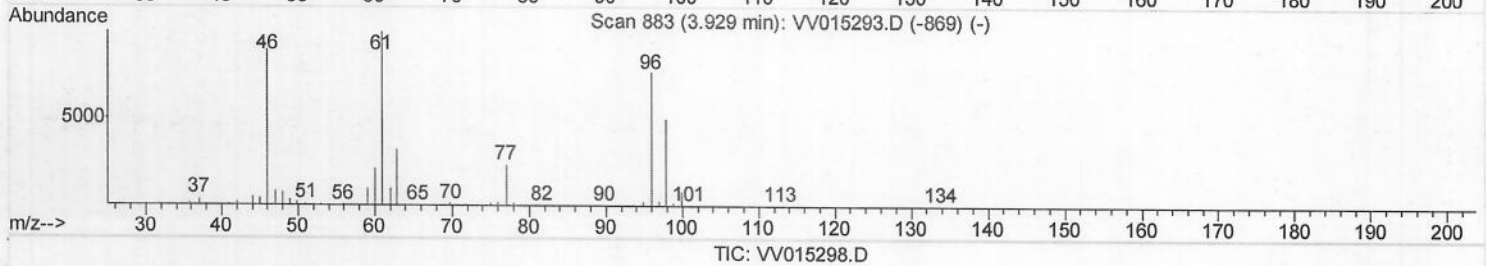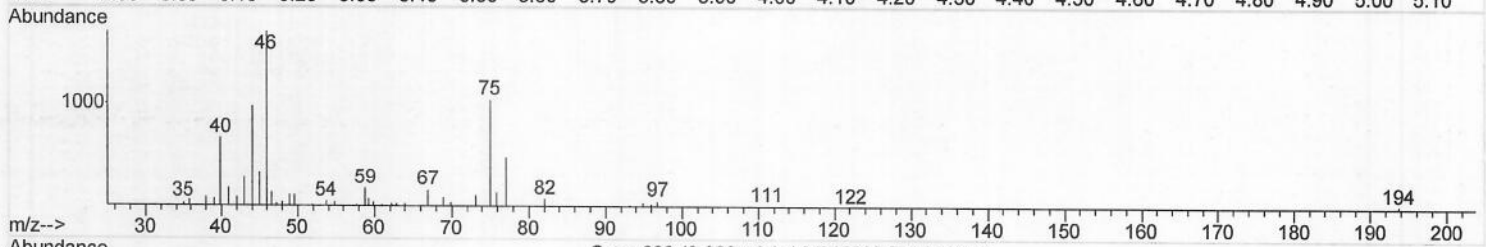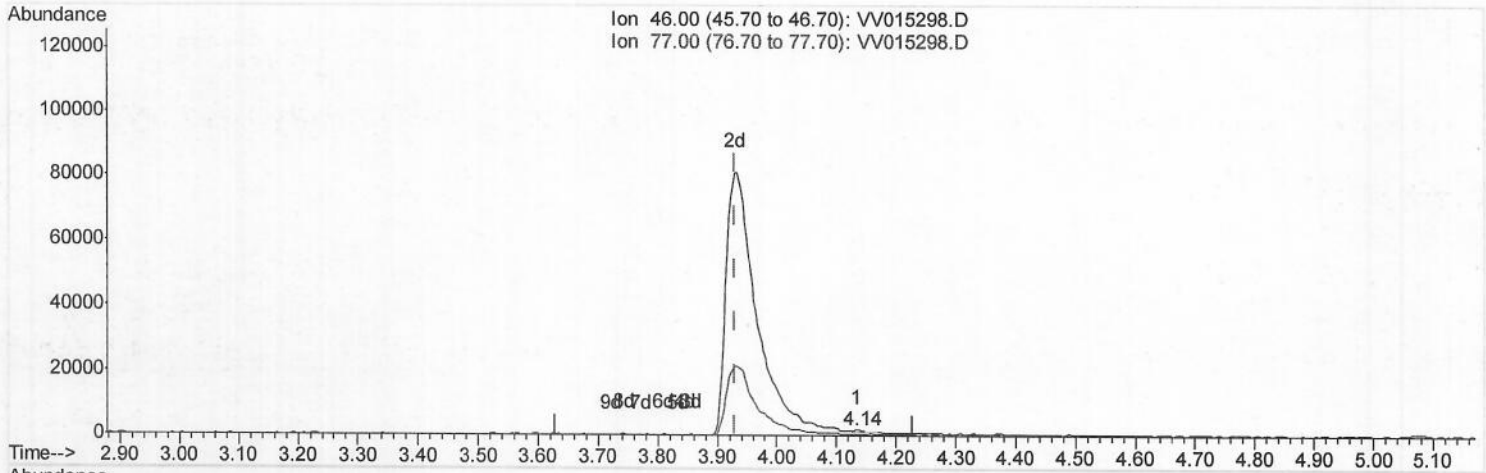

(21) 2-Butanone-d5 (S)

4.135min (+0.206) 0.36ug/L

response 984

Ion	Exp%	Act%
46.00	100	100
77.00	10.70	13.11
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015298.D
 Acq On : 31 Mar 2020 02:36
 Operator : SY/MD
 Sample : L1975-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:21:17 PM

Quant Time: Mar 31 06:28:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 06:20:52 2020
 Response via : Initial Calibration

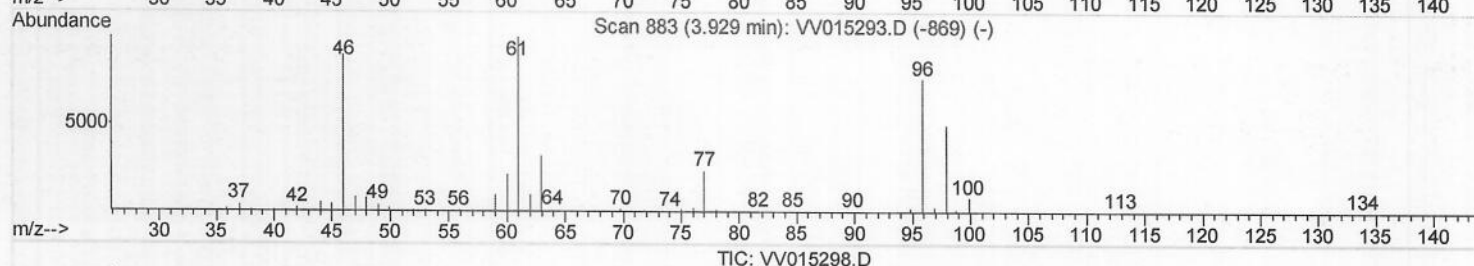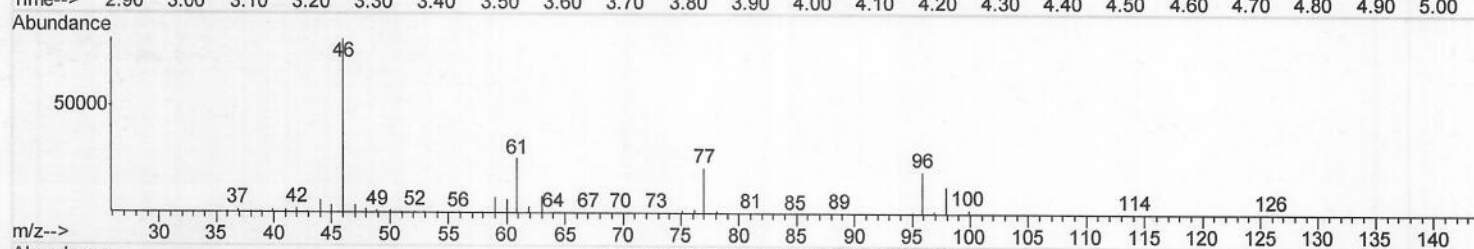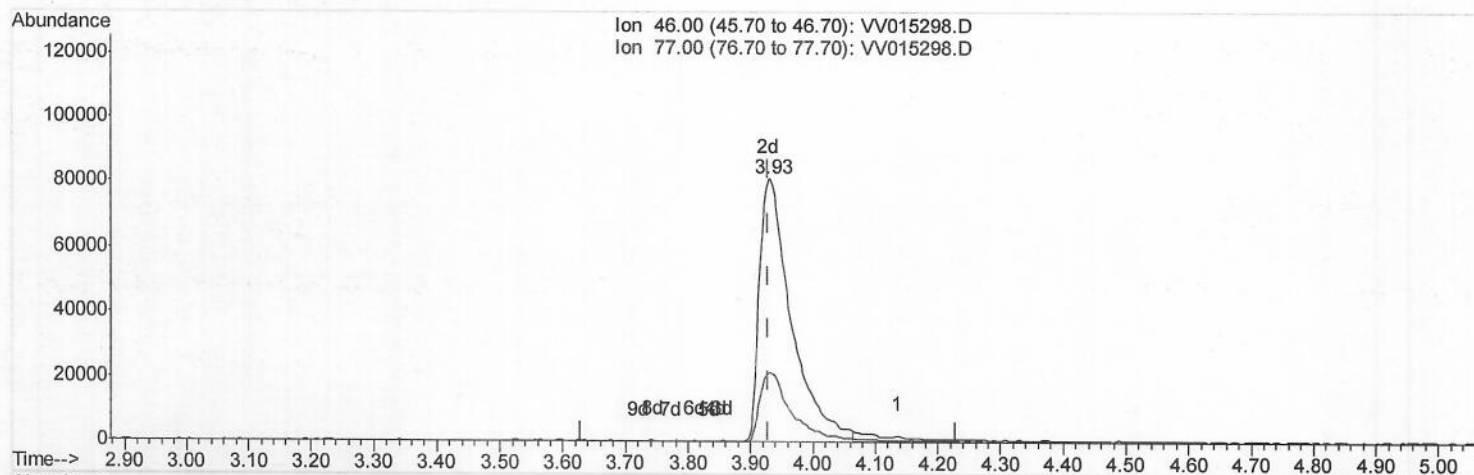

(21) 2-Butanone-d5 (S)

3.929min (+0.000) 107.16ug/L m >

response 292363

Ion	Exp%	Act%
46.00	100	100
77.00	10.70	0.04#
0.00	0.00	0.00
0.00	0.00	0.00

MD
 04/2/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015298.D
 Acq On : 31 Mar 2020 02:36
 Operator : SY/MD
 Sample : L1975-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:21:17 PM

Quant Time: Mar 31 06:48:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 06:20:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	572145	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	548056	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	232713	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	204600	49.05	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	98.10%		
7) Chloroethane-d5	1.58	69	195209	50.28	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	100.56%		
11) 1,1-Dichloroethene-d2	2.12	63	319310	35.49	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.98%		
21) 2-Butanone-d5	3.93	46	292363m	107.16	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	107.16%		
24) Chloroform-d	4.38	84	369732	49.30	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.60%		
26) 1,2-Dichloroethane-d4	5.06	65	259396	52.92	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.84%		
32) Benzene-d6	5.08	84	745552	52.11	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.22%		
36) 1,2-Dichloropropane-d6	6.09	67	235281	52.59	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	105.18%		
41) Toluene-d8	7.34	98	711339	51.39	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.78%		
43) trans-1,3-Dichloropropene-	7.64	79	119814	49.18	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	98.36%		
47) 2-Hexanone-d5	8.12	63	236434	112.65	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	112.65%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	336363	50.94	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	101.88%		
64) 1,2-Dichlorobenzene-d4	11.65	152	239523	51.71	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.42%		
Target Compounds						
5) Vinyl chloride	1.32	62	79160	16.415	ug/L	100
20) cis-1,2-Dichloroethene	3.94	96	64092	16.079	ug/L #	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 04/2/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015298.D
 Acq On : 31 Mar 2020 02:36
 Operator : SY/MD
 Sample : L1975-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Quant Time: Mar 31 06:48:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 06:20:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 4:21:17 PM

