

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015280.D
 Acq On : 30 Mar 2020 18:30
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Quant Time: Mar 31 03:30:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 31 02:12:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	612131	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	584316	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	252617	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	206630	46.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.60%
7) Chloroethane-d5	1.58	69	226932	54.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.28%
11) 1,1-Dichloroethene-d2	2.12	63	323166	33.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.16%
21) 2-Butanone-d5	3.92	46	297514	101.93	ug/L	-0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.93%
24) Chloroform-d	4.38	84	397168	49.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.06	65	268462	51.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.38%
32) Benzene-d6	5.08	84	777905	51.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.09	67	250611	52.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.08%
41) Toluene-d8	7.34	98	749020	50.76	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.52%
43) trans-1,3-Dichloropropene-	7.64	79	126330	48.63	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.26%
47) 2-Hexanone-d5	8.11	63	266299	119.00	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	119.00%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	353073	50.16	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.32%
64) 1,2-Dichlorobenzene-d4	11.65	152	252179	50.15	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.30%


Target Compounds					Ovalue
13) Acetone	2.20	43	5253	2.637 ug/L	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015280.D
Acq On : 30 Mar 2020 18:30
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Time: Mar 31 03:30:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 31 02:12:40 2020
Response via : Initial Calibration

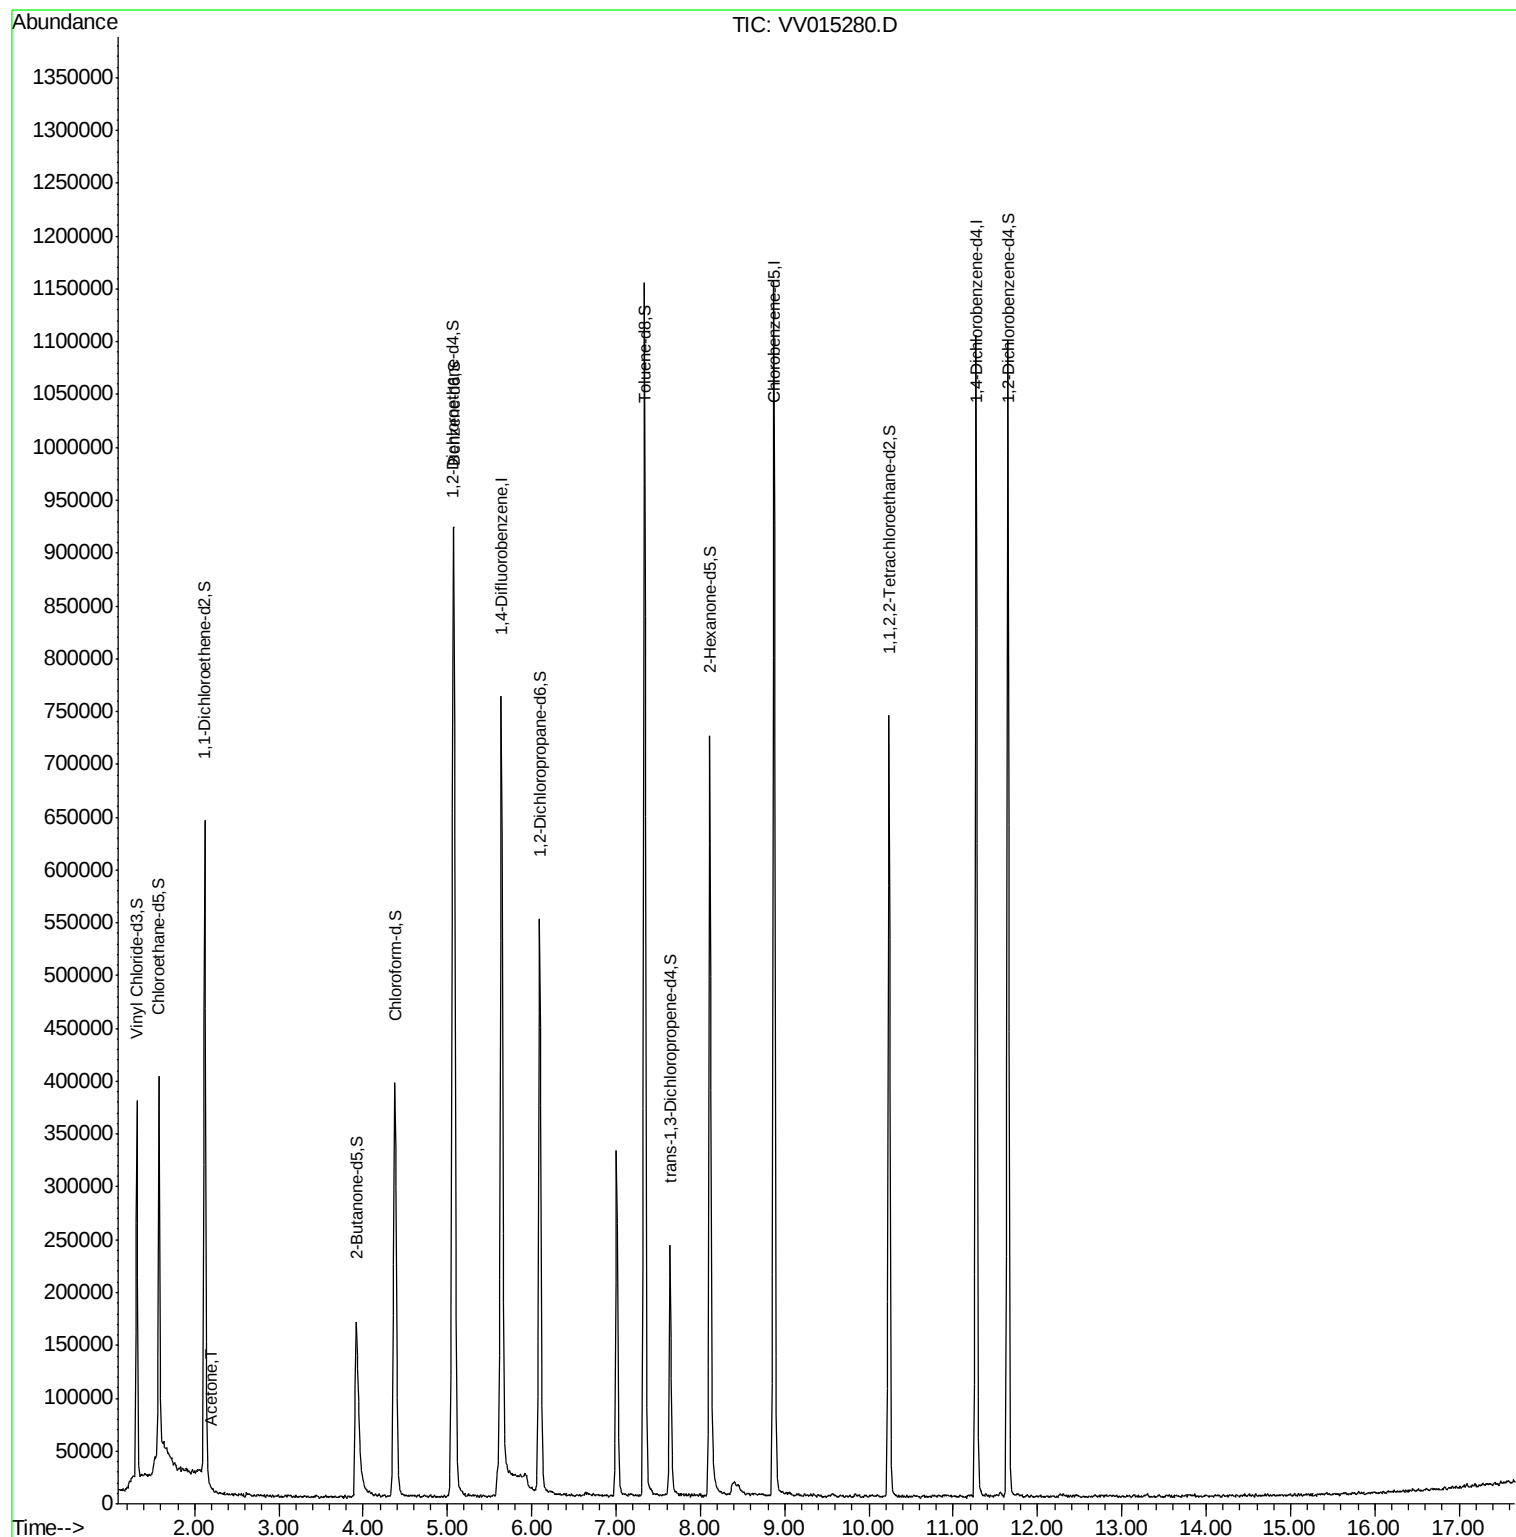

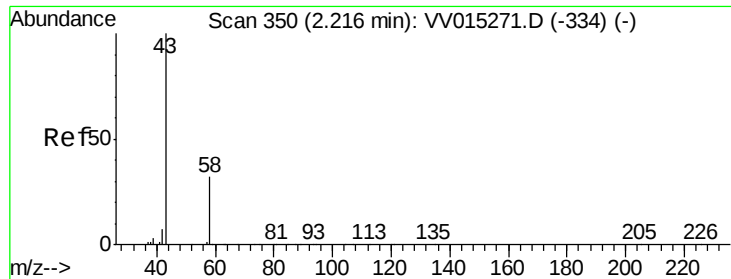

#13

Acetone

Concen: 2.637 ug/L

RT: 2.20 min Scan# 346

Delta R.T. -0.01 min

Lab File: VV015280.D

Acq: 30 Mar 2020 18:30

Instrument :

MSVOA_V

ClientSampleId :

VIBLK80

Tot Ion: 43 Resp: 5253

Ion Ratio Lower Upper

43 100

58 6.7 0.0 63.6

