

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015273.D
 Acq On : 30 Mar 2020 15:40
 Operator : SY/MD
 Sample : L2045-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	81	rVB	359358	370262	15.66%	1.838%
2	1.576	145	151	166	rBV	315204	381196	16.12%	1.892%
3	2.119	312	320	339	rVB	736360	1097390	46.41%	5.448%
4	3.116	627	630	631	rBV3	1495	821	0.03%	0.004%
5	3.508	749	752	753	rBV3	1367	929	0.04%	0.005%
6	3.531	757	759	764	rVV4	2086	1537	0.07%	0.008%
7	3.569	769	771	774	rVB4	2075	1082	0.05%	0.005%
8	3.724	816	819	821	rBV3	1847	1078	0.05%	0.005%
9	3.781	833	837	841	rBV7	2193	1507	0.06%	0.007%
10	3.817	845	848	850	rBV4	1916	1108	0.05%	0.006%
11	3.849	856	858	860	rBV3	1692	1099	0.05%	0.005%
12	3.936	873	885	934	rBV	123386	564607	23.88%	2.803%
13	4.376	1007	1022	1051	rVB	388212	963075	40.73%	4.781%
14	4.765	1139	1143	1145	rBV5	1641	1380	0.06%	0.007%
15	4.897	1180	1184	1186	rBV5	1140	835	0.04%	0.004%
16	4.910	1186	1188	1189	rBV2	1591	794	0.03%	0.004%
17	4.990	1210	1213	1217	rBV5	1360	1170	0.05%	0.006%
18	5.071	1222	1238	1265	rVV2	946398	2364598	100.00%	11.739%
19	5.640	1401	1415	1440	rBV	846230	1701989	71.98%	8.449%
20	5.990	1522	1524	1529	rBV6	1546	840	0.04%	0.004%
21	6.093	1543	1556	1579	rBV	539080	1096444	46.37%	5.443%
22	6.415	1652	1656	1660	rBV5	2202	2134	0.09%	0.011%
23	6.540	1690	1695	1699	rBV7	1494	1576	0.07%	0.008%
24	6.572	1699	1705	1708	rBV6	1876	1762	0.07%	0.009%
25	6.707	1744	1747	1749	rVB4	2380	1186	0.05%	0.006%
26	6.727	1749	1753	1754	rBV5	2334	1462	0.06%	0.007%
27	6.769	1763	1766	1768	rBV3	1250	938	0.04%	0.005%
28	6.785	1768	1771	1772	rBV3	2010	1240	0.05%	0.006%
29	6.968	1825	1828	1829	rBV3	1329	745	0.03%	0.004%
30	7.006	1830	1840	1858	rVV	337736	602056	25.46%	2.989%
31	7.219	1903	1906	1909	rVB5	2331	1487	0.06%	0.007%
32	7.338	1931	1943	1961	rBV	1172197	2016510	85.28%	10.011%
33	7.643	2028	2038	2063	rVB2	232538	398725	16.86%	1.979%
34	7.772	2075	2078	2081	rBV4	3222	2023	0.09%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015273.D
 Acq On : 30 Mar 2020 15:40
 Operator : SY/MD
 Sample : L2045-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	8.045	2159	2163	2166	rBV5	1893	1611	0.07%	0.008%
36	8.067	2169	2170	2173	rBV3	1625	1015	0.04%	0.005%
37	8.116	2175	2185	2215	rBV2	636627	1314411	55.59%	6.525%
38	8.505	2304	2306	2309	rBV3	1761	876	0.04%	0.004%
39	8.733	2375	2377	2386	rVB9	2105	2308	0.10%	0.011%
40	8.875	2408	2421	2443	rBV	1309865	2135971	90.33%	10.604%
41	9.235	2531	2533	2538	rVB6	1811	1372	0.06%	0.007%
42	9.408	2584	2587	2590	rBV4	1812	1680	0.07%	0.008%
43	9.466	2602	2605	2608	rVB5	1565	1098	0.05%	0.005%
44	9.521	2616	2622	2623	rBV4	1573	1057	0.04%	0.005%
45	9.559	2630	2634	2635	rBV4	2136	1483	0.06%	0.007%
46	9.701	2674	2678	2681	rBV5	1537	1189	0.05%	0.006%
47	9.730	2681	2687	2691	rVB8	3259	3121	0.13%	0.015%
48	9.749	2691	2693	2696	rBV4	1509	998	0.04%	0.005%
49	9.884	2732	2735	2737	rBV3	1785	961	0.04%	0.005%
50	9.936	2749	2751	2753	rBV3	1525	884	0.04%	0.004%
51	10.022	2776	2778	2780	rBV3	1628	966	0.04%	0.005%
52	10.109	2801	2805	2808	rVB6	1689	1133	0.05%	0.006%
53	10.157	2813	2820	2824	rBV10	2509	2915	0.12%	0.014%
54	10.238	2833	2845	2864	rBV	761213	1185083	50.12%	5.883%
55	10.334	2873	2875	2877	rBV3	1740	814	0.03%	0.004%
56	10.350	2877	2880	2883	rVB5	2581	1838	0.08%	0.009%
57	10.370	2883	2886	2891	rBV7	1645	1466	0.06%	0.007%
58	10.418	2896	2901	2903	rBV6	1859	1977	0.08%	0.010%
59	10.466	2914	2916	2919	rBV4	1224	870	0.04%	0.004%
60	10.556	2941	2944	2949	rBV6	2792	2294	0.10%	0.011%
61	10.710	2986	2992	2995	rBV8	2771	2356	0.10%	0.012%
62	10.759	3004	3007	3010	rBV4	1933	1096	0.05%	0.005%
63	10.778	3010	3013	3017	rVB4	3587	2903	0.12%	0.014%
64	10.797	3017	3019	3021	rBV3	2116	1270	0.05%	0.006%
65	10.884	3044	3046	3048	rVB3	2117	862	0.04%	0.004%
66	10.916	3055	3056	3058	rBV2	1408	792	0.03%	0.004%
67	11.026	3087	3090	3094	rVB6	2019	1246	0.05%	0.006%
68	11.087	3103	3109	3112	rBV7	3289	2408	0.10%	0.012%
69	11.128	3118	3122	3125	rBV5	1616	1227	0.05%	0.006%
70	11.273	3155	3167	3183	rBV	1317742	2035715	86.09%	10.106%
71	11.476	3227	3230	3232	rBV4	1785	1037	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015273.D
 Acq On : 30 Mar 2020 15:40
 Operator : SY/MD
 Sample : L2045-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.646	3272	3283	3301	rBV	1136617	1778034	75.19%	8.827%
73	12.087	3417	3420	3422	rVB4	1986	1177	0.05%	0.006%
74	12.106	3422	3426	3431	rBV8	2381	3028	0.13%	0.015%
75	12.132	3431	3434	3437	rVV5	1533	858	0.04%	0.004%
76	12.180	3444	3449	3451	rBV6	2583	1851	0.08%	0.009%
77	12.225	3457	3463	3465	rBV7	2081	1691	0.07%	0.008%
78	12.276	3476	3479	3484	rVB5	2104	1727	0.07%	0.009%
79	12.344	3494	3500	3503	rBV7	2279	2556	0.11%	0.013%
80	12.360	3503	3505	3507	rVV3	1884	826	0.03%	0.004%
81	12.559	3565	3567	3570	rVB4	2277	1287	0.05%	0.006%
82	12.588	3570	3576	3578	rBV7	2687	2760	0.12%	0.014%
83	12.665	3594	3600	3601	rBV5	5269	4440	0.19%	0.022%
84	12.784	3634	3637	3639	rBV4	1275	772	0.03%	0.004%
85	12.797	3639	3641	3645	rVB4	2806	1525	0.06%	0.008%
86	12.823	3645	3649	3651	rBV5	1874	1560	0.07%	0.008%
87	13.161	3751	3754	3757	rBV3	1507	1012	0.04%	0.005%
88	13.238	3776	3778	3781	rBV4	1923	831	0.04%	0.004%
89	13.289	3785	3794	3803	rBV4	7981	13844	0.59%	0.069%
90	13.463	3842	3848	3850	rBV6	3326	2585	0.11%	0.013%
91	13.505	3855	3861	3862	rBV5	2104	1898	0.08%	0.009%
92	13.749	3931	3937	3939	rBV6	3063	2665	0.11%	0.013%
93	13.839	3962	3965	3968	rBV5	2039	1677	0.07%	0.008%
94	14.038	4024	4027	4031	rBV5	2104	1884	0.08%	0.009%
95	14.058	4031	4033	4037	rBV3	1495	1150	0.05%	0.006%
96	14.170	4065	4068	4070	rBV3	2181	1451	0.06%	0.007%
97	14.241	4088	4090	4094	rBV5	1385	816	0.03%	0.004%
98	14.389	4134	4136	4139	rBV3	1569	907	0.04%	0.005%
99	14.517	4174	4176	4178	rBV3	2161	1314	0.06%	0.007%
100	14.749	4245	4248	4251	rBV4	2162	1709	0.07%	0.008%


Sum of corrected areas: 20143723

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015273.D
Acq On : 30 Mar 2020 15:40
Operator : SY/MD
Sample : L2045-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

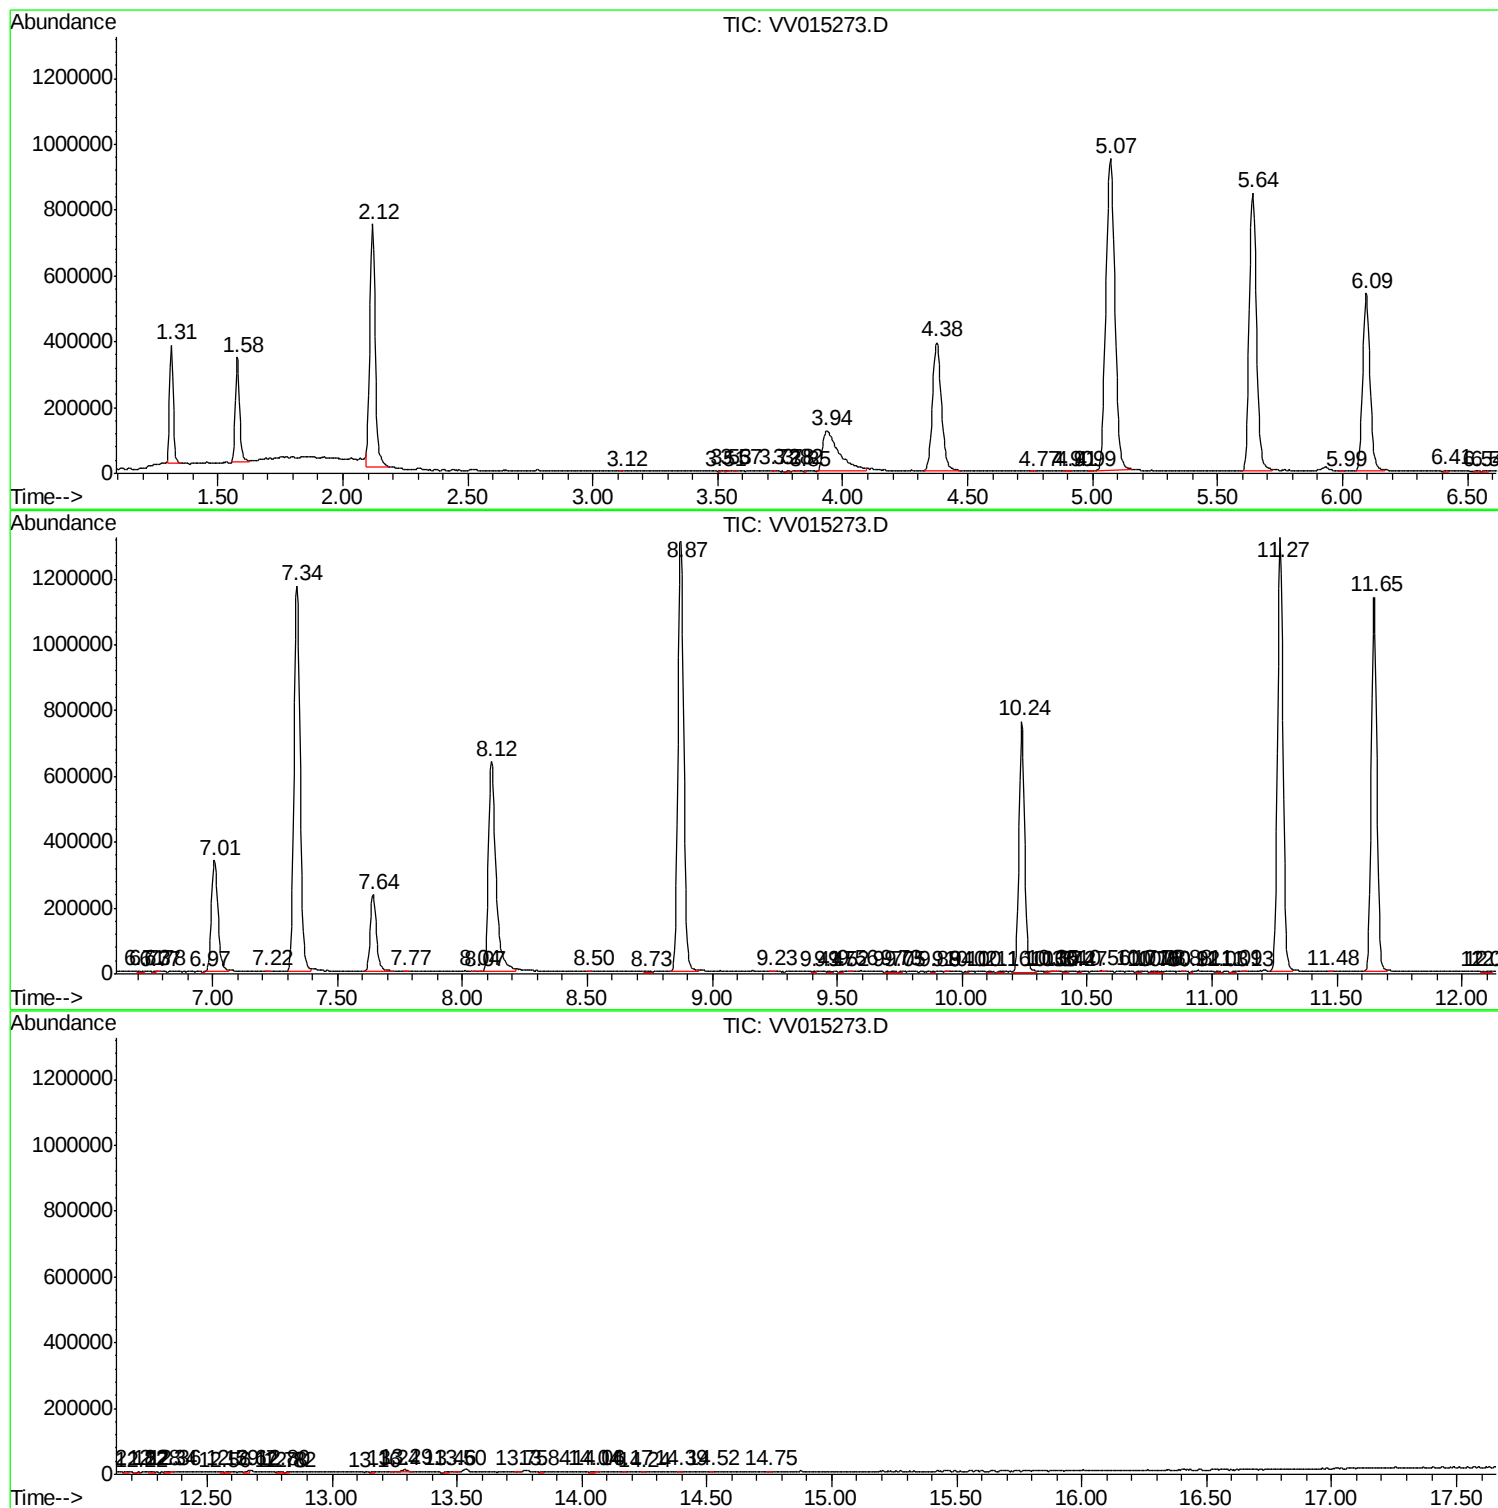

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015273.D
Acq On : 30 Mar 2020 15:40
Operator : SY/MD
Sample : L2045-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015273.D
Acq On : 30 Mar 2020 15:40
Operator : SY/MD
Sample : L2045-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc