

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015274.D
 Acq On : 30 Mar 2020 16:05
 Operator : SY/MD
 Sample : L1941-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	353412	354005	16.04%	1.946%
2	1.579	146	152	165	rVB	300962	351261	15.91%	1.931%
3	2.119	313	320	332	rVB	654774	914396	41.42%	5.028%
4	2.717	503	506	507	rBV2	2123	1319	0.06%	0.007%
5	3.267	675	677	681	rBV4	1833	1372	0.06%	0.008%
6	3.302	686	688	690	rBV4	1537	674	0.03%	0.004%
7	3.389	710	715	719	rBV6	1794	2067	0.09%	0.011%
8	3.405	719	720	722	rBV2	1235	612	0.03%	0.003%
9	3.502	748	750	755	rVB5	1731	1017	0.05%	0.006%
10	3.560	765	768	771	rVB4	1516	1036	0.05%	0.006%
11	3.576	771	773	774	rBV2	1373	519	0.02%	0.003%
12	3.691	807	809	811	rBV2	1585	1011	0.05%	0.006%
13	3.759	829	830	833	rBV3	1306	723	0.03%	0.004%
14	3.878	863	867	868	rBV4	1343	958	0.04%	0.005%
15	3.942	875	887	935	rBV2	112576	520012	23.56%	2.859%
16	4.380	1008	1023	1047	rVB2	358029	892076	40.41%	4.905%
17	4.601	1089	1092	1094	rBV3	1604	833	0.04%	0.005%
18	4.817	1157	1159	1160	rVB2	1451	519	0.02%	0.003%
19	4.833	1160	1164	1168	rBV7	1792	1397	0.06%	0.008%
20	4.987	1210	1212	1216	rBV4	1541	928	0.04%	0.005%
21	5.074	1222	1239	1275	rVB2	884548	2207419	100.00%	12.137%
22	5.643	1403	1416	1443	rBV	720653	1443405	65.39%	7.936%
23	5.933	1494	1506	1517	rBV	11734	28636	1.30%	0.157%
24	6.013	1528	1531	1535	rBV4	2389	1317	0.06%	0.007%
25	6.097	1544	1557	1578	rBV	500057	1005669	45.56%	5.529%
26	6.643	1724	1727	1728	rBV3	1657	940	0.04%	0.005%
27	6.791	1770	1773	1775	rBV4	1931	1214	0.05%	0.007%
28	6.855	1790	1793	1795	rBV3	2662	1858	0.08%	0.010%
29	6.894	1803	1805	1808	rBV3	1575	895	0.04%	0.005%
30	6.949	1820	1822	1825	rVB4	1935	861	0.04%	0.005%
31	7.010	1828	1841	1859	rBV	313917	565459	25.62%	3.109%
32	7.148	1881	1884	1887	rBV4	1885	1439	0.07%	0.008%
33	7.338	1931	1943	1964	rBV	1067419	1835702	83.16%	10.093%
34	7.643	2028	2038	2062	rBV	215286	373366	16.91%	2.053%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015274.D
 Acq On : 30 Mar 2020 16:05
 Operator : SY/MD
 Sample : L1941-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	7.833	2095	2097	2102	rVB5	2254	1435	0.07%	0.008%
36	7.913	2121	2122	2125	rVB3	1223	584	0.03%	0.003%
37	7.929	2125	2127	2130	rBV3	1025	628	0.03%	0.003%
38	8.116	2175	2185	2216	rBV2	616152	1281393	58.05%	7.045%
39	8.357	2256	2260	2261	rBV4	1983	1385	0.06%	0.008%
40	8.521	2310	2311	2313	rBV2	1268	536	0.02%	0.003%
41	8.723	2370	2374	2378	rBV7	2180	1935	0.09%	0.011%
42	8.797	2394	2397	2401	rVB4	1669	1149	0.05%	0.006%
43	8.826	2401	2406	2408	rBV6	2679	2048	0.09%	0.011%
44	8.875	2408	2421	2443	rBV	1119899	1820262	82.46%	10.008%
45	9.164	2508	2511	2514	rBV5	2619	2073	0.09%	0.011%
46	9.392	2578	2582	2583	rBV3	1377	1012	0.05%	0.006%
47	9.453	2597	2601	2608	rBV8	2038	2354	0.11%	0.013%
48	9.524	2619	2623	2625	rBV4	1611	1134	0.05%	0.006%
49	9.608	2647	2649	2652	rBV4	1689	1408	0.06%	0.008%
50	9.649	2657	2662	2663	rBV5	1147	1143	0.05%	0.006%
51	9.739	2687	2690	2691	rBV3	1045	552	0.03%	0.003%
52	9.781	2700	2703	2706	rBV5	2664	2265	0.10%	0.012%
53	9.871	2728	2731	2735	rVV5	2144	1471	0.07%	0.008%
54	9.903	2738	2741	2747	rVB7	1214	1011	0.05%	0.006%
55	9.932	2747	2750	2755	rBV6	1884	1943	0.09%	0.011%
56	9.981	2763	2765	2767	rBV3	1104	526	0.02%	0.003%
57	10.051	2785	2787	2792	rBB5	1627	1287	0.06%	0.007%
58	10.161	2818	2821	2822	rBV	1525	955	0.04%	0.005%
59	10.238	2829	2845	2865	rBV	719460	1142098	51.74%	6.280%
60	10.428	2902	2904	2906	rBV3	1102	538	0.02%	0.003%
61	10.508	2927	2929	2930	rBV2	1241	612	0.03%	0.003%
62	10.624	2963	2965	2968	rVB3	1938	693	0.03%	0.004%
63	10.714	2989	2993	2996	rBV5	1965	1325	0.06%	0.007%
64	10.862	3037	3039	3040	rBV2	1246	577	0.03%	0.003%
65	10.929	3055	3060	3061	rBV5	1607	1158	0.05%	0.006%
66	11.006	3079	3084	3087	rBV6	1925	2239	0.10%	0.012%
67	11.148	3125	3128	3130	rBV3	1903	1172	0.05%	0.006%
68	11.186	3137	3140	3141	rBV3	2743	1775	0.08%	0.010%
69	11.273	3155	3167	3185	rBV	1112654	1696907	76.87%	9.330%
70	11.466	3224	3227	3228	rBV3	1308	574	0.03%	0.003%
71	11.508	3237	3240	3243	rBV5	1785	1122	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015274.D
 Acq On : 30 Mar 2020 16:05
 Operator : SY/MD
 Sample : L1941-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.563	3249	3257	3258	rBV10	2067	2023	0.09%	0.011%
73	11.649	3272	3284	3306	rBV	1070999	1644303	74.49%	9.041%
74	11.845	3343	3345	3347	rBV3	1157	633	0.03%	0.003%
75	12.132	3433	3434	3436	rBV2	1245	668	0.03%	0.004%
76	12.161	3441	3443	3446	rVB4	1571	760	0.03%	0.004%
77	12.183	3448	3450	3452	rVB3	1916	756	0.03%	0.004%
78	12.260	3471	3474	3477	rBV4	2080	1758	0.08%	0.010%
79	12.289	3480	3483	3486	rVB5	1686	865	0.04%	0.005%
80	12.360	3504	3505	3508	rBV3	1869	1015	0.05%	0.006%
81	12.392	3513	3515	3518	rVV4	1947	1057	0.05%	0.006%
82	12.418	3521	3523	3527	rVB4	2314	1467	0.07%	0.008%
83	12.453	3531	3534	3538	rBV4	2459	2279	0.10%	0.013%
84	12.588	3574	3576	3578	rBV3	1315	506	0.02%	0.003%
85	12.675	3595	3603	3612	rBV3	5214	8275	0.37%	0.045%
86	12.807	3640	3644	3646	rBV5	1942	1548	0.07%	0.009%
87	12.907	3673	3675	3678	rVB4	1364	752	0.03%	0.004%
88	12.935	3678	3684	3686	rBV7	1841	2240	0.10%	0.012%
89	13.013	3706	3708	3710	rBV3	1950	1036	0.05%	0.006%
90	13.112	3734	3739	3742	rBV6	2241	1884	0.09%	0.010%
91	13.170	3754	3757	3759	rBV3	1484	898	0.04%	0.005%
92	13.196	3759	3765	3766	rBV5	2713	2359	0.11%	0.013%
93	13.334	3804	3808	3813	rVB6	2229	1959	0.09%	0.011%
94	13.373	3818	3820	3828	rVB9	2266	2861	0.13%	0.016%
95	13.820	3955	3959	3962	rBV6	1408	998	0.05%	0.005%
96	13.839	3962	3965	3967	rVB3	2360	1395	0.06%	0.008%
97	13.868	3971	3974	3978	rBV4	2508	2162	0.10%	0.012%
98	13.939	3993	3996	3999	rBV5	2062	1889	0.09%	0.010%
99	14.032	4022	4025	4029	rBV5	2536	1706	0.08%	0.009%
100	14.955	4310	4312	4315	rBV4	2056	1285	0.06%	0.007%


Sum of corrected areas: 18187531

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015274.D
Acq On : 30 Mar 2020 16:05
Operator : SY/MD
Sample : L1941-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

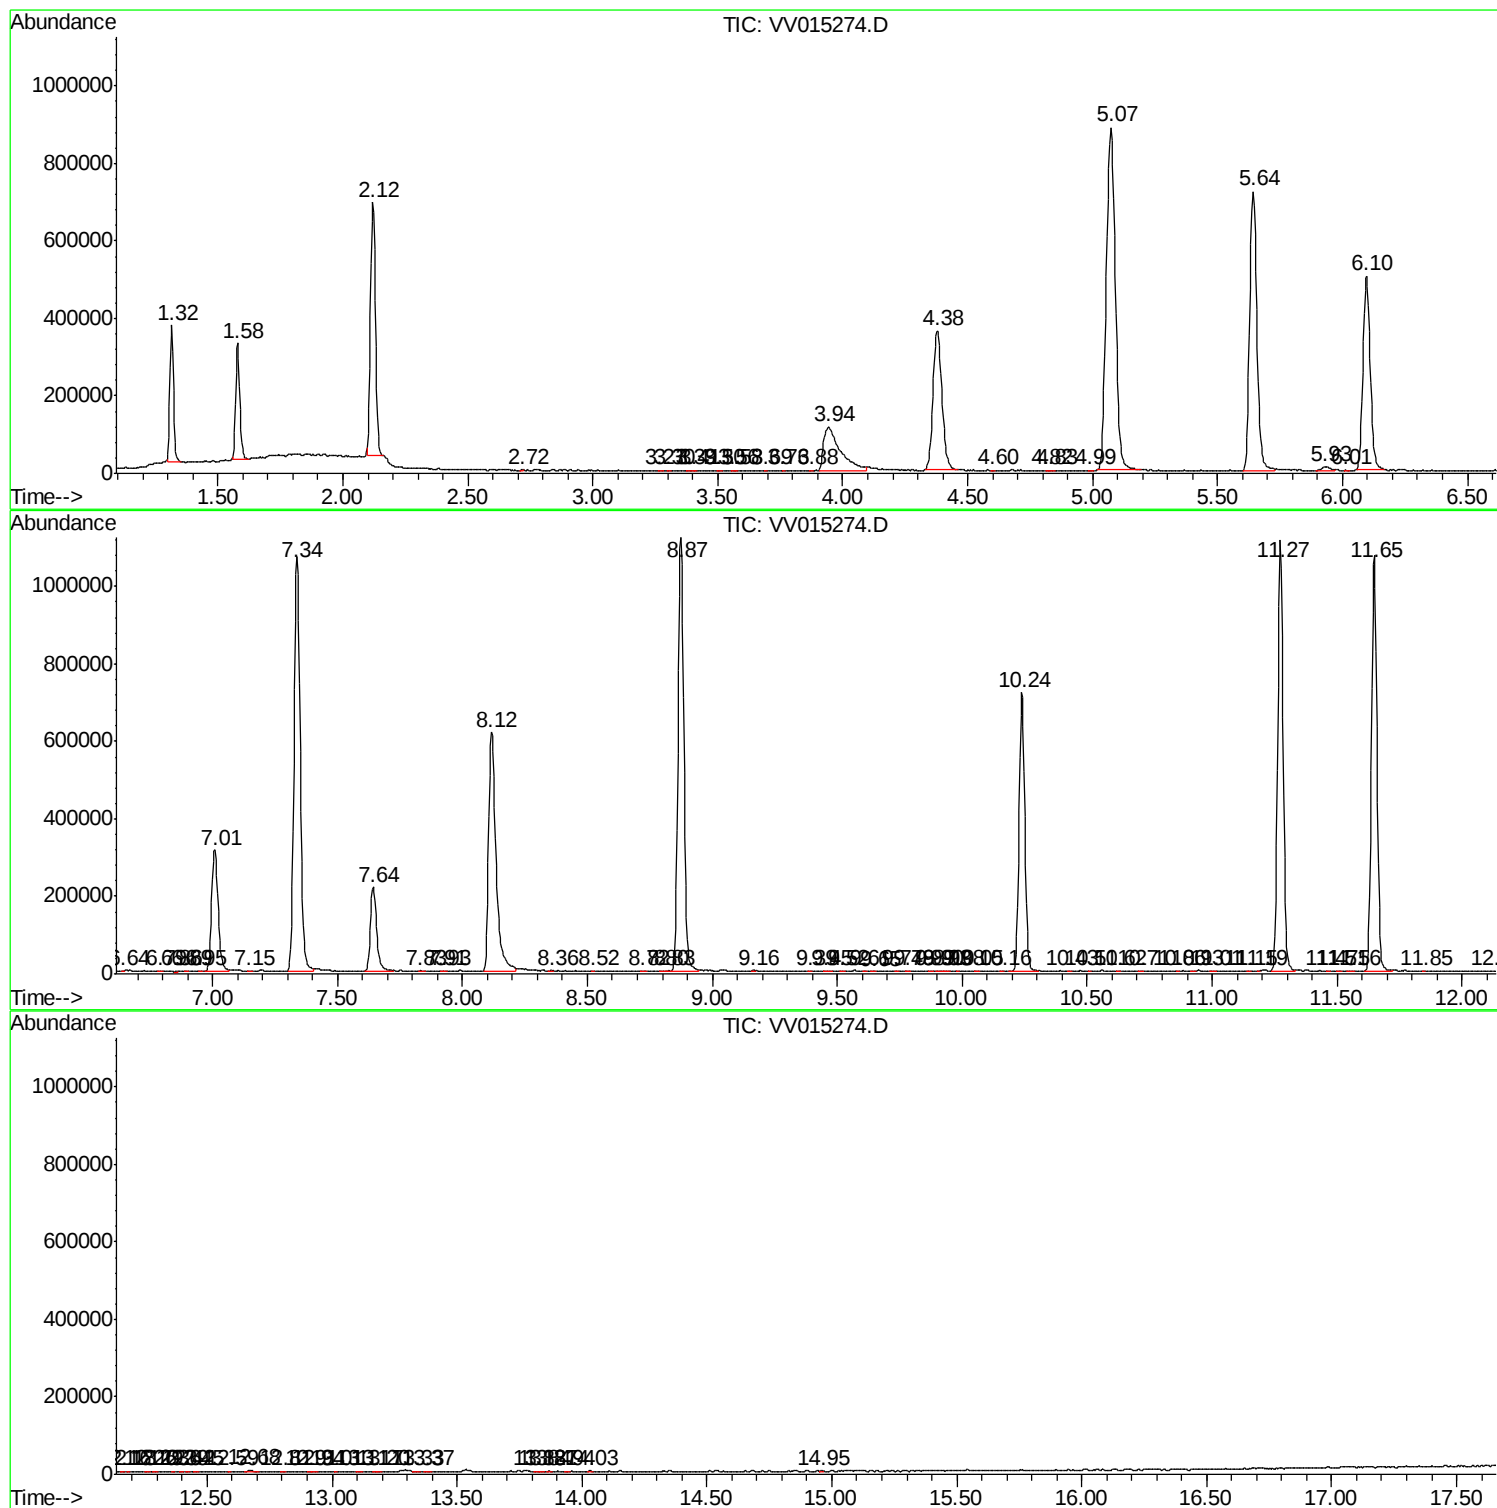

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015274.D
Acq On : 30 Mar 2020 16:05
Operator : SY/MD
Sample : L1941-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015274.D
Acq On : 30 Mar 2020 16:05
Operator : SY/MD
Sample : L1941-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc