

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015275.D
 Acq On : 30 Mar 2020 16:29
 Operator : SY/MD
 Sample : L1968-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	337179	348228	15.32%	1.848%
2	1.579	146	152	163	rVB	295585	340520	14.98%	1.807%
3	2.119	313	320	332	rVB	647971	906175	39.86%	4.809%
4	2.836	541	543	545	rBV3	1794	1015	0.04%	0.005%
5	2.965	580	583	584	rBV3	1682	919	0.04%	0.005%
6	3.084	618	620	623	rBV4	2911	1717	0.08%	0.009%
7	3.126	631	633	634	rBV2	1127	555	0.02%	0.003%
8	3.200	654	656	657	rBV2	1712	673	0.03%	0.004%
9	3.222	661	663	665	rBV2	1647	545	0.02%	0.003%
10	3.235	665	667	670	rVB3	1679	822	0.04%	0.004%
11	3.360	704	706	708	rBV3	1620	876	0.04%	0.005%
12	3.502	748	750	753	rBV4	1221	715	0.03%	0.004%
13	3.576	770	773	781	rBV7	1782	1994	0.09%	0.011%
14	3.730	818	821	823	rVB4	2165	1253	0.06%	0.007%
15	3.759	825	830	834	rVV8	2301	2536	0.11%	0.013%
16	3.782	834	837	840	rVV5	1525	1099	0.05%	0.006%
17	3.820	846	849	852	rBV4	2355	1712	0.08%	0.009%
18	3.859	858	861	866	rVB5	1499	999	0.04%	0.005%
19	3.881	866	868	871	rBV3	911	545	0.02%	0.003%
20	3.936	871	885	927	rBV2	128497	565443	24.87%	3.001%
21	4.376	1007	1022	1052	rVB	374509	933777	41.07%	4.956%
22	4.737	1131	1134	1137	rBV5	1388	1152	0.05%	0.006%
23	4.807	1154	1156	1158	rBV4	1678	625	0.03%	0.003%
24	4.836	1163	1165	1169	rVB3	1910	1091	0.05%	0.006%
25	5.074	1222	1239	1264	rBV2	905756	2273608	100.00%	12.067%
26	5.643	1403	1416	1437	rBV	747838	1483493	65.25%	7.873%
27	5.846	1477	1479	1482	rBV3	2476	1565	0.07%	0.008%
28	6.097	1544	1557	1580	rBV	514471	1040412	45.76%	5.522%
29	6.367	1639	1641	1643	rBV4	1357	651	0.03%	0.003%
30	6.466	1670	1672	1673	rBV2	1216	543	0.02%	0.003%
31	6.544	1694	1696	1698	rBV3	1259	670	0.03%	0.004%
32	6.569	1702	1704	1708	rVB5	2141	1288	0.06%	0.007%
33	6.589	1708	1710	1711	rBV2	2144	903	0.04%	0.005%
34	6.855	1789	1793	1795	rBV4	1461	1029	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015275.D
 Acq On : 30 Mar 2020 16:29
 Operator : SY/MD
 Sample : L1968-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	6.872	1795	1798	1800	rBV4	2237	1256	0.06%	0.007%
36	6.955	1822	1824	1826	rVB3	1857	945	0.04%	0.005%
37	7.010	1826	1841	1862	rBV	321154	591170	26.00%	3.138%
38	7.338	1931	1943	1965	rBV	1110222	1908206	83.93%	10.127%
39	7.643	2025	2038	2058	rBV	224669	390892	17.19%	2.075%
40	8.029	2156	2158	2161	rVB3	1858	631	0.03%	0.003%
41	8.116	2174	2185	2223	rBV2	657460	1382590	60.81%	7.338%
42	8.415	2274	2278	2281	rBV6	2712	2771	0.12%	0.015%
43	8.608	2332	2338	2340	rBV7	2219	2229	0.10%	0.012%
44	8.698	2364	2366	2369	rVB4	1777	709	0.03%	0.004%
45	8.736	2376	2378	2380	rBV3	1444	617	0.03%	0.003%
46	8.765	2384	2387	2394	rVB9	2061	1612	0.07%	0.009%
47	8.807	2394	2400	2402	rBV6	2298	2213	0.10%	0.012%
48	8.875	2409	2421	2444	rBV	1149387	1892510	83.24%	10.044%
49	9.093	2487	2489	2492	rBV4	1516	860	0.04%	0.005%
50	9.244	2534	2536	2537	rBV2	1450	562	0.02%	0.003%
51	9.357	2568	2571	2573	rBV4	1983	1082	0.05%	0.006%
52	9.389	2578	2581	2585	rBV5	1741	1092	0.05%	0.006%
53	9.518	2619	2621	2623	rBV3	1394	591	0.03%	0.003%
54	9.701	2674	2678	2681	rBV7	1307	1320	0.06%	0.007%
55	9.778	2699	2702	2703	rBV3	1094	643	0.03%	0.003%
56	9.826	2715	2717	2719	rBV3	1879	891	0.04%	0.005%
57	9.875	2730	2732	2735	rVB3	1394	928	0.04%	0.005%
58	9.894	2735	2738	2742	rBV6	2564	1968	0.09%	0.010%
59	9.929	2745	2749	2750	rVB4	1086	651	0.03%	0.003%
60	9.942	2750	2753	2756	rBV4	1913	1737	0.08%	0.009%
61	10.016	2775	2776	2778	rBV2	1656	892	0.04%	0.005%
62	10.084	2795	2797	2800	rBV4	1612	1062	0.05%	0.006%
63	10.109	2803	2805	2807	rBV3	1843	728	0.03%	0.004%
64	10.177	2818	2826	2832	rBV3	1472	2478	0.11%	0.013%
65	10.238	2832	2845	2859	rBV	752000	1190491	52.36%	6.318%
66	10.469	2915	2917	2919	rBV3	1464	772	0.03%	0.004%
67	10.489	2921	2923	2924	rBV2	1444	580	0.03%	0.003%
68	10.630	2964	2967	2971	rVV5	2148	1720	0.08%	0.009%
69	10.736	2998	3000	3005	rVB5	1863	1316	0.06%	0.007%
70	10.759	3005	3007	3011	rBV5	1659	1431	0.06%	0.008%
71	10.791	3014	3017	3020	rBV5	1293	974	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015275.D
 Acq On : 30 Mar 2020 16:29
 Operator : SY/MD
 Sample : L1968-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.013	3083	3086	3087	rBV3	1233	710	0.03%	0.004%
73	11.164	3131	3133	3135	rBV3	1295	556	0.02%	0.003%
74	11.193	3139	3142	3143	rBV3	2915	1752	0.08%	0.009%
75	11.273	3155	3167	3190	rBV	1140905	1773054	77.98%	9.410%
76	11.650	3272	3284	3301	rBV	1105784	1718012	75.56%	9.118%
77	12.000	3390	3393	3395	rBV3	1704	891	0.04%	0.005%
78	12.093	3419	3422	3427	rBV6	1707	1571	0.07%	0.008%
79	12.125	3430	3432	3440	rVB8	2111	2305	0.10%	0.012%
80	12.158	3440	3442	3445	rVB4	1551	889	0.04%	0.005%
81	12.186	3445	3451	3452	rBV6	2102	2321	0.10%	0.012%
82	12.222	3459	3462	3463	rBV3	1318	671	0.03%	0.004%
83	12.402	3515	3518	3524	rVB8	4305	2996	0.13%	0.016%
84	12.428	3524	3526	3528	rBV2	1966	1058	0.05%	0.006%
85	12.569	3568	3570	3578	rVB8	2512	3006	0.13%	0.016%
86	12.604	3578	3581	3584	rBV4	1920	1285	0.06%	0.007%
87	12.649	3593	3595	3598	rBV3	2134	1488	0.07%	0.008%
88	12.720	3614	3617	3621	rBV5	2322	1873	0.08%	0.010%
89	12.746	3621	3625	3627	rBV5	2024	1417	0.06%	0.008%
90	12.823	3648	3649	3652	rBV3	1223	583	0.03%	0.003%
91	12.958	3689	3691	3693	rBV3	1633	849	0.04%	0.005%
92	13.006	3704	3706	3708	rVB3	1774	602	0.03%	0.003%
93	13.093	3731	3733	3736	rBV4	1386	705	0.03%	0.004%
94	13.264	3784	3786	3787	rBV2	1345	559	0.02%	0.003%
95	13.379	3817	3822	3825	rVB6	2230	2257	0.10%	0.012%
96	13.424	3833	3836	3840	rBV4	2004	1801	0.08%	0.010%
97	14.350	4122	4124	4127	rVB3	1385	585	0.03%	0.003%
98	14.408	4139	4142	4144	rBV3	2380	1730	0.08%	0.009%
99	14.598	4196	4201	4202	rBV4	1914	1627	0.07%	0.009%
100	15.138	4363	4369	4370	rBV5	2489	2539	0.11%	0.013%


Sum of corrected areas: 18841960

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015275.D
Acq On : 30 Mar 2020 16:29
Operator : SY/MD
Sample : L1968-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

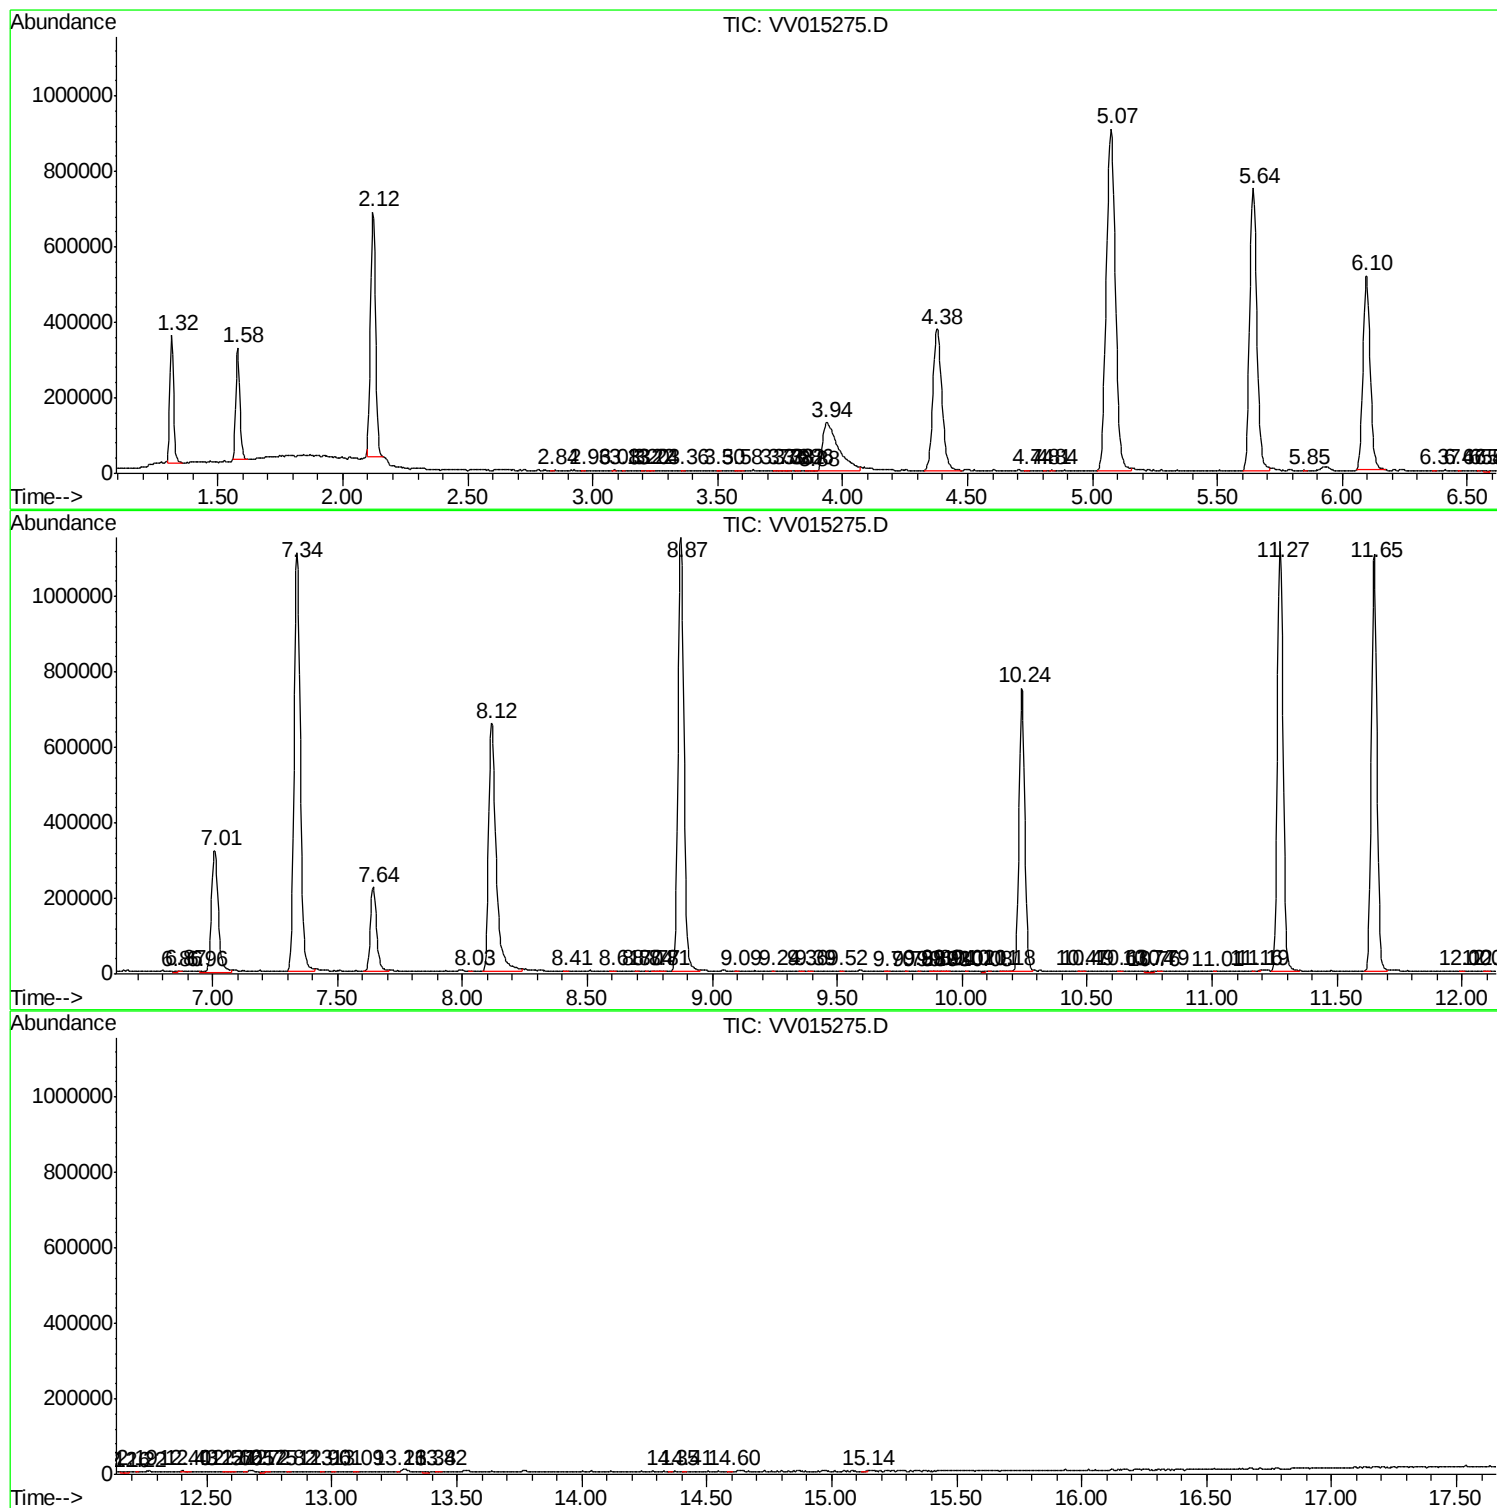

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015275.D
Acq On : 30 Mar 2020 16:29
Operator : SY/MD
Sample : L1968-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015275.D
Acq On : 30 Mar 2020 16:29
Operator : SY/MD
Sample : L1968-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc