

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015276.D
 Acq On : 30 Mar 2020 16:53
 Operator : SY/MD
 Sample : L1975-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	212313	210478	12.62%	1.611%
2	1.579	146	152	163	rBV	179535	210606	12.63%	1.612%
3	2.119	313	320	348	rVB	372214	604190	36.23%	4.624%
4	3.045	603	608	609	rBV5	2391	1873	0.11%	0.014%
5	3.109	626	628	633	rBV4	2337	1655	0.10%	0.013%
6	3.306	687	689	692	rBV4	1653	947	0.06%	0.007%
7	3.476	740	742	743	rBV2	1245	466	0.03%	0.004%
8	3.486	743	745	747	rBV3	1921	1016	0.06%	0.008%
9	3.569	768	771	774	rBV3	1954	1042	0.06%	0.008%
10	3.688	806	808	809	rBV2	746	207	0.01%	0.002%
11	3.701	809	812	815	rBV4	2497	1562	0.09%	0.012%
12	3.820	847	849	853	rBV6	1934	1333	0.08%	0.010%
13	3.939	875	886	922	rBV2	98011	378081	22.67%	2.893%
14	4.380	1009	1023	1045	rVB2	244142	599255	35.93%	4.586%
15	4.772	1143	1145	1148	rVB4	1772	804	0.05%	0.006%
16	4.949	1198	1200	1203	rBV3	1509	852	0.05%	0.007%
17	5.074	1222	1239	1269	rBV2	565261	1432361	85.88%	10.961%
18	5.495	1367	1370	1371	rBV3	1719	987	0.06%	0.008%
19	5.643	1403	1416	1446	rBV	664299	1332459	79.89%	10.197%
20	6.032	1535	1537	1540	rBV3	1756	1275	0.08%	0.010%
21	6.096	1545	1557	1578	rVB	340186	686555	41.16%	5.254%
22	6.318	1624	1626	1627	rBV2	1213	520	0.03%	0.004%
23	6.556	1697	1700	1701	rBV2	1399	677	0.04%	0.005%
24	6.743	1756	1758	1759	rBV2	1378	544	0.03%	0.004%
25	6.788	1771	1772	1775	rVB3	1654	859	0.05%	0.007%
26	6.839	1785	1788	1792	rBV5	2313	1712	0.10%	0.013%
27	6.878	1798	1800	1803	rBV3	1269	790	0.05%	0.006%
28	7.010	1830	1841	1863	rBV	158843	291783	17.49%	2.233%
29	7.180	1892	1894	1896	rBV3	1779	878	0.05%	0.007%
30	7.338	1932	1943	1961	rBV	627874	1084482	65.02%	8.299%
31	7.598	2021	2024	2025	rBV2	1918	1120	0.07%	0.009%
32	7.643	2029	2038	2055	rVV	116540	199971	11.99%	1.530%
33	8.119	2174	2186	2215	rBV2	418490	893137	53.55%	6.835%
34	8.547	2317	2319	2323	rBV5	1814	1058	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015276.D
 Acq On : 30 Mar 2020 16:53
 Operator : SY/MD
 Sample : L1975-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	8.707	2365	2369	2371	rBV5	1556	1123	0.07%	0.009%
36	8.874	2408	2421	2442	rBV	1034623	1667841	100.00%	12.763%
37	9.231	2530	2532	2535	rBV4	1939	946	0.06%	0.007%
38	9.264	2540	2542	2543	rBV3	1199	505	0.03%	0.004%
39	9.402	2582	2585	2586	rBV3	2225	1155	0.07%	0.009%
40	9.476	2603	2608	2610	rBV5	2844	2240	0.13%	0.017%
41	9.492	2610	2613	2615	rBV4	1376	914	0.05%	0.007%
42	9.585	2640	2642	2646	rBV5	2137	1880	0.11%	0.014%
43	9.659	2662	2665	2668	rVB3	1805	1284	0.08%	0.010%
44	9.682	2668	2672	2674	rBV5	1709	1491	0.09%	0.011%
45	9.714	2680	2682	2683	rBV3	1135	451	0.03%	0.003%
46	9.746	2690	2692	2693	rBV2	1083	596	0.04%	0.005%
47	9.813	2709	2713	2714	rBV4	1984	1233	0.07%	0.009%
48	9.858	2722	2727	2731	rBV7	1553	1412	0.08%	0.011%
49	10.026	2776	2779	2782	rBV4	2026	1789	0.11%	0.014%
50	10.109	2801	2805	2808	rBV5	1929	1847	0.11%	0.014%
51	10.193	2828	2831	2833	rBV4	1456	828	0.05%	0.006%
52	10.241	2834	2846	2868	rVV	516840	812693	48.73%	6.219%
53	10.444	2908	2909	2913	rBV4	1267	717	0.04%	0.005%
54	10.527	2933	2935	2937	rBV3	1200	625	0.04%	0.005%
55	10.633	2966	2968	2969	rBV2	1530	761	0.05%	0.006%
56	10.678	2979	2982	2983	rBV3	1643	1191	0.07%	0.009%
57	10.772	3006	3011	3013	rBV5	2403	1956	0.12%	0.015%
58	10.794	3016	3018	3020	rVV3	1248	460	0.03%	0.004%
59	10.871	3038	3042	3043	rBV4	1965	1599	0.10%	0.012%
60	10.907	3051	3053	3055	rBV3	676	264	0.02%	0.002%
61	11.090	3108	3110	3113	rVB4	1655	748	0.04%	0.006%
62	11.148	3124	3128	3130	rBV4	1497	1067	0.06%	0.008%
63	11.273	3154	3167	3187	rBV	970174	1502167	90.07%	11.495%
64	11.649	3272	3284	3299	rBV	693119	1088472	65.26%	8.330%
65	11.820	3335	3337	3340	rBV4	1686	1004	0.06%	0.008%
66	11.964	3379	3382	3385	rBV4	2334	1908	0.11%	0.015%
67	12.029	3400	3402	3406	rBV4	1557	1258	0.08%	0.010%
68	12.180	3448	3449	3450	rBV	776	176	0.01%	0.001%
69	12.196	3450	3454	3455	rBV3	2664	1705	0.10%	0.013%
70	12.337	3496	3498	3502	rVB3	2527	1805	0.11%	0.014%
71	12.360	3502	3505	3507	rBV4	1661	1313	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015276.D
Acq On : 30 Mar 2020 16:53
Operator : SY/MD
Sample : L1975-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Title : VOC Analysis

72	12.395	3514	3516	3518	rBV3	1449	546	0.03%	0.004%
73	12.434	3522	3528	3529	rBV5	2593	2190	0.13%	0.017%
74	12.501	3547	3549	3550	rBV	904	473	0.03%	0.004%
75	12.749	3624	3626	3630	rBV4	1373	1105	0.07%	0.008%
76	13.398	3826	3828	3830	rBV3	1656	978	0.06%	0.007%
77	13.437	3838	3840	3841	rBV2	1241	501	0.03%	0.004%
78	13.697	3918	3921	3926	rBV6	1550	1600	0.10%	0.012%
79	14.180	4069	4071	4073	rBV3	1805	1063	0.06%	0.008%
80	14.318	4112	4114	4116	rBV2	2350	1307	0.08%	0.010%
81	14.768	4252	4254	4263	rVB9	2692	2875	0.17%	0.022%


Sum of corrected areas: 13067597

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015276.D
Acq On : 30 Mar 2020 16:53
Operator : SY/MD
Sample : L1975-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

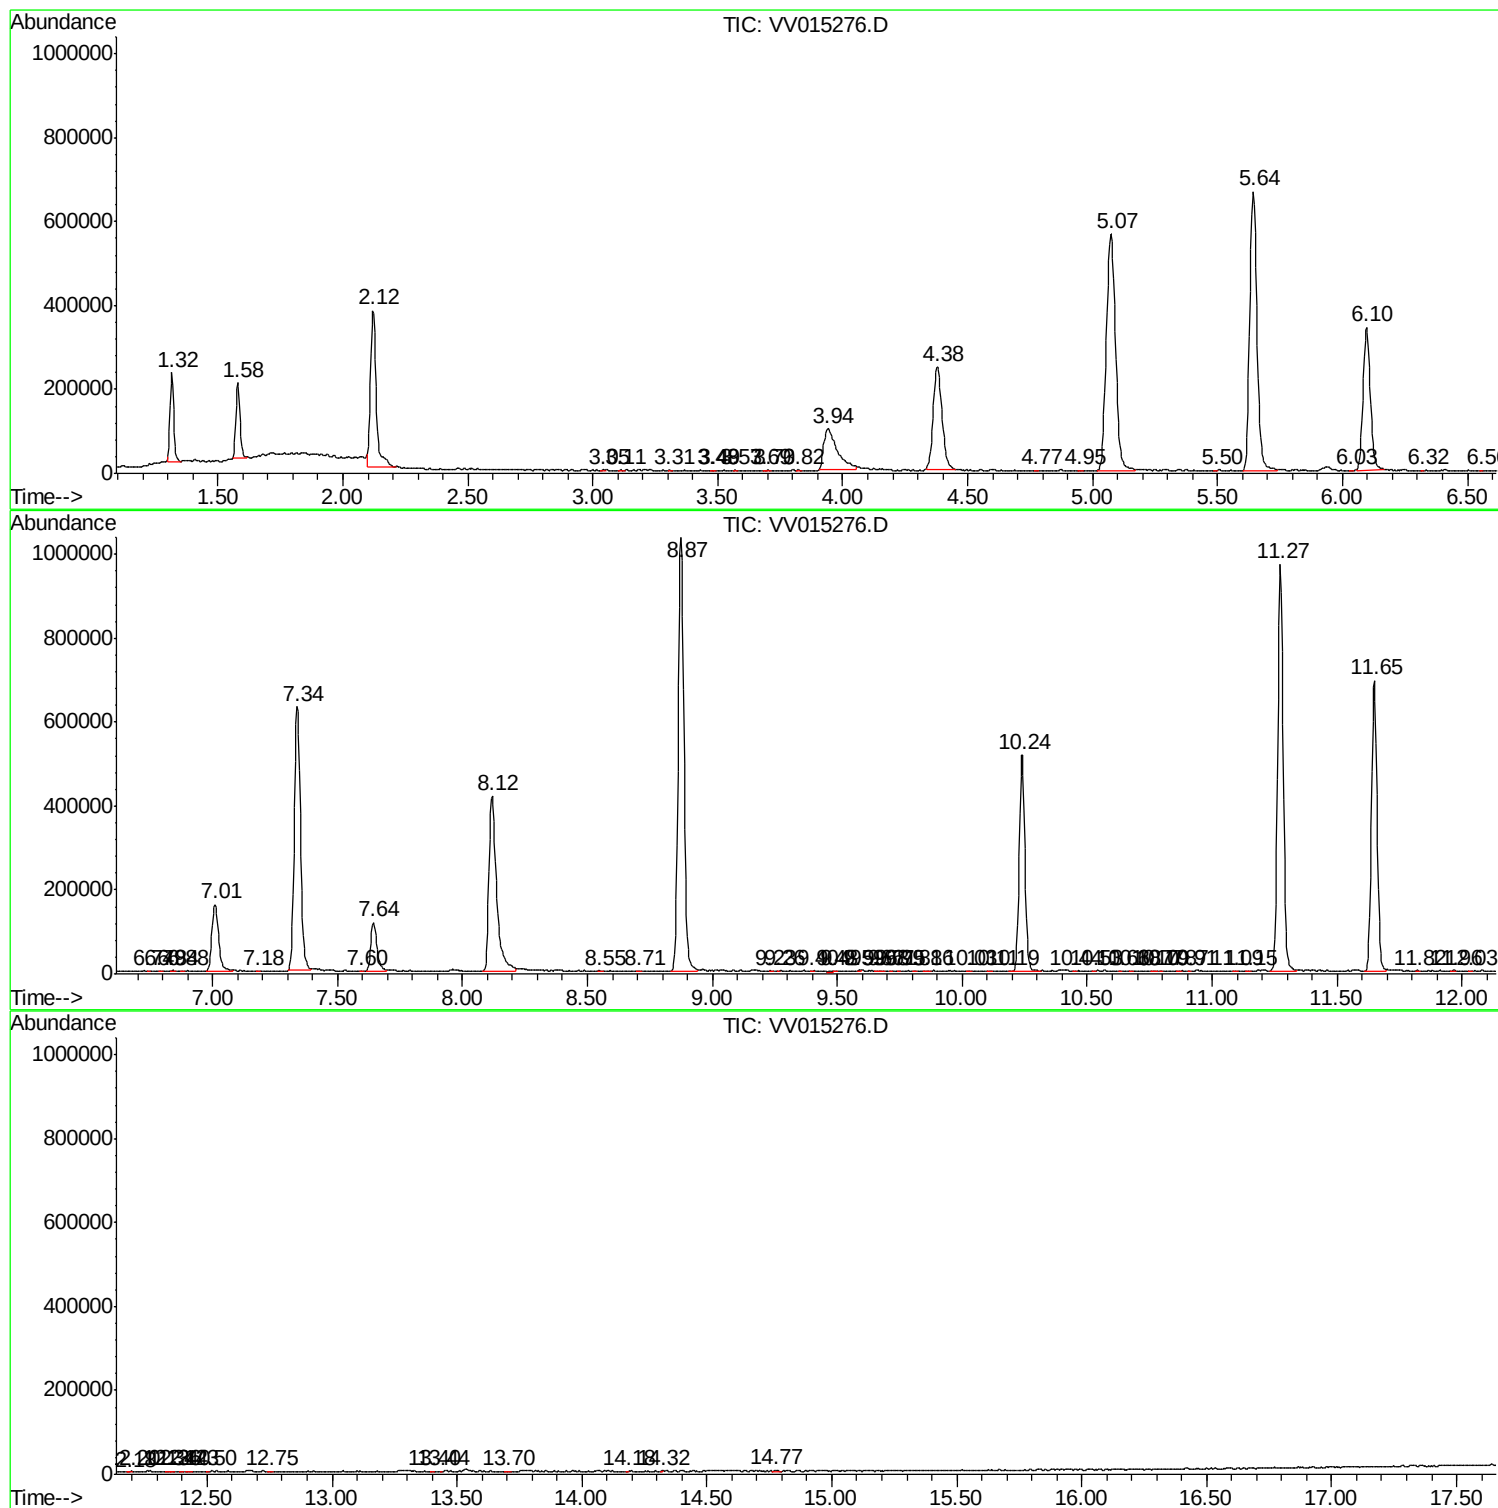

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015276.D
Acq On : 30 Mar 2020 16:53
Operator : SY/MD
Sample : L1975-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033020\
Data File : VV015276.D
Acq On : 30 Mar 2020 16:53
Operator : SY/MD
Sample : L1975-21
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
