

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015280.D
 Acq On : 30 Mar 2020 18:30
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	355067	352752	15.15%	1.854%
2	1.579	146	152	162	rVB	346950	397874	17.08%	2.091%
3	2.122	313	321	345	rVB	632141	955417	41.02%	5.021%
4	2.859	546	550	554	rBV6	2259	1934	0.08%	0.010%
5	2.929	567	572	577	rVB9	2022	2490	0.11%	0.013%
6	2.955	577	580	582	rBV4	1487	1053	0.05%	0.006%
7	3.019	596	600	603	rBV5	1536	1558	0.07%	0.008%
8	3.293	680	685	687	rBV5	1582	1433	0.06%	0.008%
9	3.341	697	700	705	rVB7	1910	1663	0.07%	0.009%
10	3.367	705	708	711	rBV3	827	735	0.03%	0.004%
11	3.418	721	724	727	rBV4	1398	1065	0.05%	0.006%
12	3.437	728	730	731	rBV2	1425	537	0.02%	0.003%
13	3.495	744	748	749	rBV4	1133	801	0.03%	0.004%
14	3.531	756	759	763	rBV5	1775	1358	0.06%	0.007%
15	3.556	763	767	770	rVB6	1701	1347	0.06%	0.007%
16	3.592	776	778	781	rBV3	1175	593	0.03%	0.003%
17	3.614	783	785	788	rVB4	1818	1058	0.05%	0.006%
18	3.637	790	792	795	rBV4	1116	617	0.03%	0.003%
19	3.666	798	801	808	rVB9	1805	1726	0.07%	0.009%
20	3.698	808	811	812	rBV3	1037	549	0.02%	0.003%
21	3.714	814	816	819	rVB4	1642	616	0.03%	0.003%
22	3.765	829	832	834	rVB4	1433	812	0.03%	0.004%
23	3.785	834	838	844	rVB8	3262	2973	0.13%	0.016%
24	3.817	844	848	849	rBV4	2081	1354	0.06%	0.007%
25	3.920	869	880	912	rBV2	164769	514653	22.10%	2.705%
26	4.376	1009	1022	1047	rVB	389904	939974	40.36%	4.940%
27	4.643	1102	1105	1108	rBV4	2129	1467	0.06%	0.008%
28	4.707	1121	1125	1127	rBV3	1492	1158	0.05%	0.006%
29	4.823	1158	1161	1164	rVB4	1442	845	0.04%	0.004%
30	4.846	1166	1168	1173	rVB5	2157	1073	0.05%	0.006%
31	4.868	1173	1175	1178	rBV4	1717	848	0.04%	0.004%
32	4.900	1183	1185	1188	rBV4	1146	624	0.03%	0.003%
33	4.942	1196	1198	1201	rVB4	1449	511	0.02%	0.003%
34	4.958	1201	1203	1204	rBV2	1975	894	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015280.D
 Acq On : 30 Mar 2020 18:30
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	5.074	1222	1239	1261	rBV2	916902	2328951	100.00%	12.239%
36	5.389	1333	1337	1341	rBV6	2310	2107	0.09%	0.011%
37	5.486	1361	1367	1368	rBV4	1885	1774	0.08%	0.009%
38	5.540	1380	1384	1386	rBV4	1507	1287	0.06%	0.007%
39	5.640	1394	1415	1441	rBV	756951	1666473	71.55%	8.758%
40	6.093	1545	1556	1575	rVB	539239	1065228	45.74%	5.598%
41	6.759	1761	1763	1765	rBV3	1702	937	0.04%	0.005%
42	7.006	1828	1840	1858	rBV	326916	586746	25.19%	3.084%
43	7.338	1931	1943	1963	rBV	1147351	1981810	85.09%	10.415%
44	7.643	2029	2038	2057	rVB	234238	382107	16.41%	2.008%
45	8.026	2154	2157	2160	rBV4	2298	1736	0.07%	0.009%
46	8.042	2160	2162	2163	rBV2	1345	515	0.02%	0.003%
47	8.074	2169	2172	2173	rBV2	3029	1793	0.08%	0.009%
48	8.112	2173	2184	2210	rVV	719163	1283319	55.10%	6.744%
49	8.874	2409	2421	2442	rBV	1148759	1837951	78.92%	9.659%
50	9.344	2565	2567	2578	rVB10	3825	4617	0.20%	0.024%
51	9.389	2578	2581	2583	rBV4	2757	2022	0.09%	0.011%
52	9.453	2599	2601	2605	rBV4	1425	1138	0.05%	0.006%
53	9.772	2694	2700	2703	rBV6	2685	2765	0.12%	0.015%
54	9.807	2706	2711	2712	rBV4	1791	1442	0.06%	0.008%
55	10.161	2819	2821	2822	rVB2	1595	575	0.02%	0.003%
56	10.173	2822	2825	2827	rBV4	1621	1300	0.06%	0.007%
57	10.238	2834	2845	2861	rBV	738103	1167626	50.14%	6.136%
58	10.328	2871	2873	2876	rVB3	2228	1143	0.05%	0.006%
59	10.363	2882	2884	2886	rBV3	1220	792	0.03%	0.004%
60	10.440	2905	2908	2909	rBV2	1671	963	0.04%	0.005%
61	10.524	2929	2934	2935	rBV5	2008	1513	0.06%	0.008%
62	10.633	2960	2968	2970	rBV8	2087	2764	0.12%	0.015%
63	10.675	2977	2981	2984	rBV5	2004	1572	0.07%	0.008%
64	10.871	3040	3042	3044	rBV3	2142	1375	0.06%	0.007%
65	11.058	3098	3100	3103	rBV4	1346	901	0.04%	0.005%
66	11.144	3125	3127	3130	rVB4	1514	856	0.04%	0.004%
67	11.161	3130	3132	3133	rBV	2415	1175	0.05%	0.006%
68	11.270	3155	3166	3192	rBV	1100073	1725606	74.09%	9.069%
69	11.649	3272	3284	3305	rBV	1093442	1731081	74.33%	9.097%
70	11.926	3367	3370	3371	rBV3	1854	1295	0.06%	0.007%
71	12.013	3395	3397	3399	rBV3	1504	902	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015280.D
 Acq On : 30 Mar 2020 18:30
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	12.083	3416	3419	3422	rVB4	1268	808	0.03%	0.004%
73	12.106	3422	3426	3427	rBV3	1964	1536	0.07%	0.008%
74	12.144	3435	3438	3443	rBV6	1908	1914	0.08%	0.010%
75	12.177	3443	3448	3452	rBV8	1576	2002	0.09%	0.011%
76	12.212	3457	3459	3460	rBV2	1232	557	0.02%	0.003%
77	12.260	3468	3474	3475	rBV4	2982	2960	0.13%	0.016%
78	12.386	3511	3513	3515	rBV3	2252	1238	0.05%	0.007%
79	12.418	3520	3523	3525	rBV5	1999	1370	0.06%	0.007%
80	12.537	3557	3560	3565	rVB6	1857	1570	0.07%	0.008%
81	12.559	3565	3567	3569	rVV3	1543	614	0.03%	0.003%
82	12.575	3570	3572	3574	rVB3	1432	629	0.03%	0.003%
83	12.720	3615	3617	3619	rBV3	1087	613	0.03%	0.003%
84	12.755	3625	3628	3630	rBV4	2006	1146	0.05%	0.006%
85	12.939	3683	3685	3688	rVB4	1975	1008	0.04%	0.005%
86	12.964	3689	3693	3696	rVV5	1497	1047	0.04%	0.006%
87	13.141	3744	3748	3754	rVB8	2694	3313	0.14%	0.017%
88	13.167	3754	3756	3757	rBV	1509	714	0.03%	0.004%
89	13.199	3764	3766	3770	rVB5	2056	1469	0.06%	0.008%
90	13.218	3770	3772	3774	rBV3	1641	842	0.04%	0.004%
91	13.421	3832	3835	3837	rBV4	1334	926	0.04%	0.005%
92	13.476	3849	3852	3854	rBV4	1982	1100	0.05%	0.006%
93	13.582	3883	3885	3888	rBV4	1813	911	0.04%	0.005%
94	13.627	3897	3899	3902	rBV3	1704	1150	0.05%	0.006%
95	13.787	3946	3949	3950	rBV3	1773	1020	0.04%	0.005%
96	13.868	3971	3974	3976	rVB3	2993	1368	0.06%	0.007%
97	14.189	4073	4074	4077	rBV3	1387	829	0.04%	0.004%
98	14.353	4122	4125	4132	rBV7	2473	3181	0.14%	0.017%
99	14.405	4138	4141	4143	rBV3	2314	1453	0.06%	0.008%
100	15.273	4409	4411	4413	rVB2	1915	615	0.03%	0.003%


Sum of corrected areas: 19028422

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015280.D
Acq On : 30 Mar 2020 18:30
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

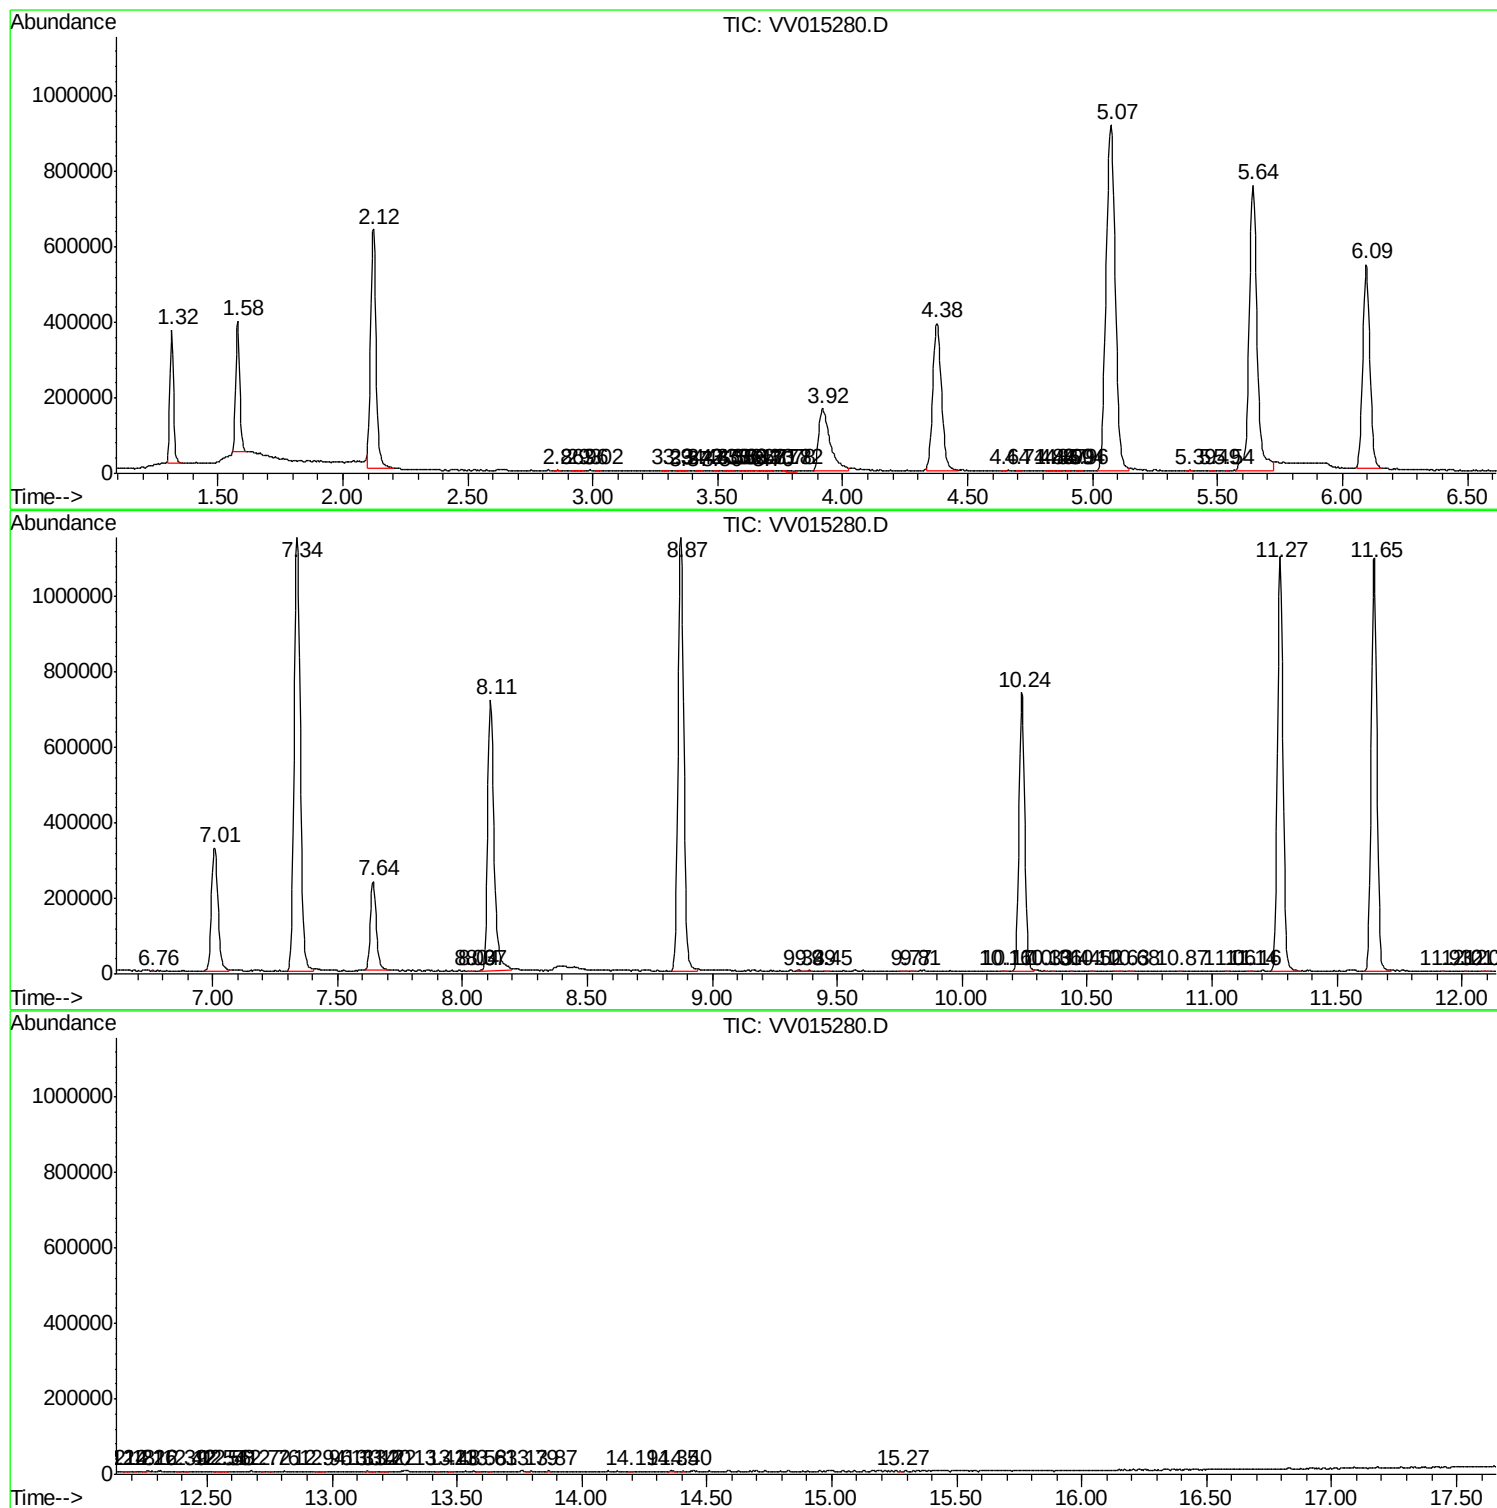

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015280.D
Acq On : 30 Mar 2020 18:30
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015280.D
Acq On : 30 Mar 2020 18:30
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc