

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015282.D
 Acq On : 30 Mar 2020 19:19
 Operator : SY/MD
 Sample : VIBLK81
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	318443	327023	14.34%	1.750%
2	1.579	147	152	170	rVB	317621	366715	16.08%	1.962%
3	2.122	313	321	344	rVB	598264	911982	39.98%	4.880%
4	2.753	515	517	522	rVB6	2348	1719	0.08%	0.009%
5	2.936	572	574	576	rBV3	1625	859	0.04%	0.005%
6	2.952	576	579	581	rVV3	1902	1146	0.05%	0.006%
7	2.994	589	592	594	rBV3	1332	990	0.04%	0.005%
8	3.042	605	607	611	rBV5	1568	763	0.03%	0.004%
9	3.126	629	633	635	rBV5	1777	1182	0.05%	0.006%
10	3.235	664	667	670	rBV5	1512	1173	0.05%	0.006%
11	3.344	699	701	704	rVB4	1597	886	0.04%	0.005%
12	3.367	704	708	710	rBV4	1246	931	0.04%	0.005%
13	3.434	725	729	733	rBV6	2237	2216	0.10%	0.012%
14	3.454	733	735	738	rVB3	1731	945	0.04%	0.005%
15	3.476	738	742	747	rBV6	1885	1889	0.08%	0.010%
16	3.515	747	754	762	rBV6	2316	3389	0.15%	0.018%
17	3.624	786	788	790	rBV3	1536	836	0.04%	0.004%
18	3.711	811	815	818	rBV5	1197	1023	0.04%	0.005%
19	3.730	818	821	824	rVB4	2423	1380	0.06%	0.007%
20	3.749	824	827	829	rBV3	2637	1592	0.07%	0.009%
21	3.817	845	848	851	rBV5	1944	1439	0.06%	0.008%
22	3.923	870	881	918	rBV2	152636	533918	23.41%	2.857%
23	4.376	1007	1022	1046	rBV2	378950	918943	40.28%	4.918%
24	4.589	1084	1088	1094	rVB8	2406	2453	0.11%	0.013%
25	4.679	1112	1116	1121	rVB7	2420	2559	0.11%	0.014%
26	4.711	1121	1126	1128	rBV5	2038	2088	0.09%	0.011%
27	4.826	1156	1162	1163	rBV6	2364	1527	0.07%	0.008%
28	4.900	1182	1185	1188	rBV4	1745	1425	0.06%	0.008%
29	4.917	1188	1190	1193	rVB3	1450	915	0.04%	0.005%
30	4.933	1193	1195	1201	rVB6	2169	1815	0.08%	0.010%
31	5.074	1218	1239	1260	rBV2	893731	2281121	100.00%	12.207%
32	5.402	1336	1341	1345	rBV8	1721	1966	0.09%	0.011%
33	5.476	1360	1364	1366	rBV4	2157	1398	0.06%	0.007%
34	5.515	1374	1376	1378	rBV3	1337	838	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015282.D
 Acq On : 30 Mar 2020 19:19
 Operator : SY/MD
 Sample : VIBLK81
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	5.592	1398	1400	1402	rBV3	1749	923	0.04%	0.005%
36	5.643	1402	1416	1435	rBV	770710	1597811	70.04%	8.550%
37	6.097	1545	1557	1579	rVB	523134	1061648	46.54%	5.681%
38	6.730	1752	1754	1757	rBV3	1098	792	0.03%	0.004%
39	6.765	1762	1765	1767	rBV4	2074	1464	0.06%	0.008%
40	7.010	1830	1841	1859	rBV	309690	552621	24.23%	2.957%
41	7.148	1882	1884	1886	rBV3	1931	858	0.04%	0.005%
42	7.235	1908	1911	1916	rBV6	2228	2294	0.10%	0.012%
43	7.338	1931	1943	1965	rBV	1102081	1901263	83.35%	10.174%
44	7.643	2028	2038	2057	rVB	221606	376250	16.49%	2.013%
45	8.113	2173	2184	2214	rBV	698582	1284413	56.31%	6.873%
46	8.875	2409	2421	2438	rBV	1165128	1883233	82.56%	10.078%
47	9.379	2575	2578	2584	rVB6	1969	1795	0.08%	0.010%
48	9.405	2584	2586	2589	rBV4	1673	1325	0.06%	0.007%
49	9.424	2589	2592	2598	rVB7	2251	2050	0.09%	0.011%
50	9.457	2598	2602	2604	rBV5	1689	1230	0.05%	0.007%
51	10.238	2833	2845	2868	rVB	743847	1164338	51.04%	6.231%
52	10.383	2886	2890	2892	rBV4	1829	1486	0.07%	0.008%
53	10.495	2922	2925	2929	rVB5	1976	1339	0.06%	0.007%
54	10.801	3017	3020	3023	rVB4	1760	1188	0.05%	0.006%
55	10.833	3027	3030	3036	rBV8	2039	1440	0.06%	0.008%
56	10.862	3036	3039	3040	rBV2	2498	1083	0.05%	0.006%
57	10.932	3058	3061	3065	rBV5	1811	1390	0.06%	0.007%
58	11.112	3115	3117	3120	rBV3	1608	1003	0.04%	0.005%
59	11.167	3132	3134	3138	rBV4	1936	1711	0.08%	0.009%
60	11.186	3138	3140	3142	rBV3	1921	1045	0.05%	0.006%
61	11.273	3154	3167	3181	rBV	1127168	1738951	76.23%	9.306%
62	11.418	3210	3212	3214	rBV3	1712	808	0.04%	0.004%
63	11.514	3239	3242	3246	rBV5	2014	1418	0.06%	0.008%
64	11.649	3271	3284	3298	rBV	1068484	1671806	73.29%	8.946%
65	11.778	3320	3324	3325	rBV4	1810	1164	0.05%	0.006%
66	11.852	3344	3347	3349	rBV4	1647	1112	0.05%	0.006%
67	11.974	3383	3385	3388	rBV3	1698	918	0.04%	0.005%
68	12.112	3425	3428	3433	rVB6	2535	2339	0.10%	0.013%
69	12.157	3440	3442	3448	rVB6	1793	1562	0.07%	0.008%
70	12.196	3453	3454	3460	rBV6	1550	1353	0.06%	0.007%
71	12.312	3488	3490	3494	rBV4	1112	1010	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015282.D
 Acq On : 30 Mar 2020 19:19
 Operator : SY/MD
 Sample : VIBLK81
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	12.331	3494	3496	3499	rVV3	2270	1186	0.05%	0.006%
73	12.350	3500	3502	3505	rVB4	1491	803	0.04%	0.004%
74	12.620	3584	3586	3588	rBV3	1776	1100	0.05%	0.006%
75	12.665	3598	3600	3601	rBV2	1967	1037	0.05%	0.006%
76	12.720	3614	3617	3620	rVB3	2210	1219	0.05%	0.007%
77	12.833	3650	3652	3655	rVB4	3104	1533	0.07%	0.008%
78	12.852	3655	3658	3662	rBV5	2064	2332	0.10%	0.012%
79	12.974	3693	3696	3699	rVB4	1505	742	0.03%	0.004%
80	13.016	3706	3709	3710	rBV2	1424	881	0.04%	0.005%
81	13.058	3719	3722	3725	rBV5	1145	737	0.03%	0.004%
82	13.074	3725	3727	3731	rVB5	1614	943	0.04%	0.005%
83	13.106	3734	3737	3739	rBV4	1799	1059	0.05%	0.006%
84	13.141	3745	3748	3752	rBV6	1827	1335	0.06%	0.007%
85	13.196	3763	3765	3769	rVB5	2052	1118	0.05%	0.006%
86	13.353	3812	3814	3818	rBV5	2611	2178	0.10%	0.012%
87	13.395	3825	3827	3832	rVB6	1346	808	0.04%	0.004%
88	13.460	3844	3847	3849	rBV4	1251	1029	0.05%	0.006%
89	13.582	3883	3885	3889	rVB5	2207	1335	0.06%	0.007%
90	13.643	3901	3904	3905	rBV3	1602	810	0.04%	0.004%
91	13.871	3972	3975	3978	rBV6	1465	737	0.03%	0.004%
92	13.939	3990	3996	4000	rVB6	2517	2545	0.11%	0.014%
93	13.964	4000	4004	4006	rBV4	2078	1496	0.07%	0.008%
94	14.013	4016	4019	4021	rBV4	1802	805	0.04%	0.004%
95	14.344	4118	4122	4123	rBV3	2118	1530	0.07%	0.008%
96	14.411	4141	4143	4148	rBV5	1556	1373	0.06%	0.007%
97	14.434	4148	4150	4152	rBV3	2214	1330	0.06%	0.007%
98	14.807	4263	4266	4268	rBV4	2257	1498	0.07%	0.008%
99	14.858	4278	4282	4284	rBV5	3013	2350	0.10%	0.013%
100	14.923	4299	4302	4306	rVB6	2386	1653	0.07%	0.009%


Sum of corrected areas: 18686980

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015282.D
Acq On : 30 Mar 2020 19:19
Operator : SY/MD
Sample : VIBLK81
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK81

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

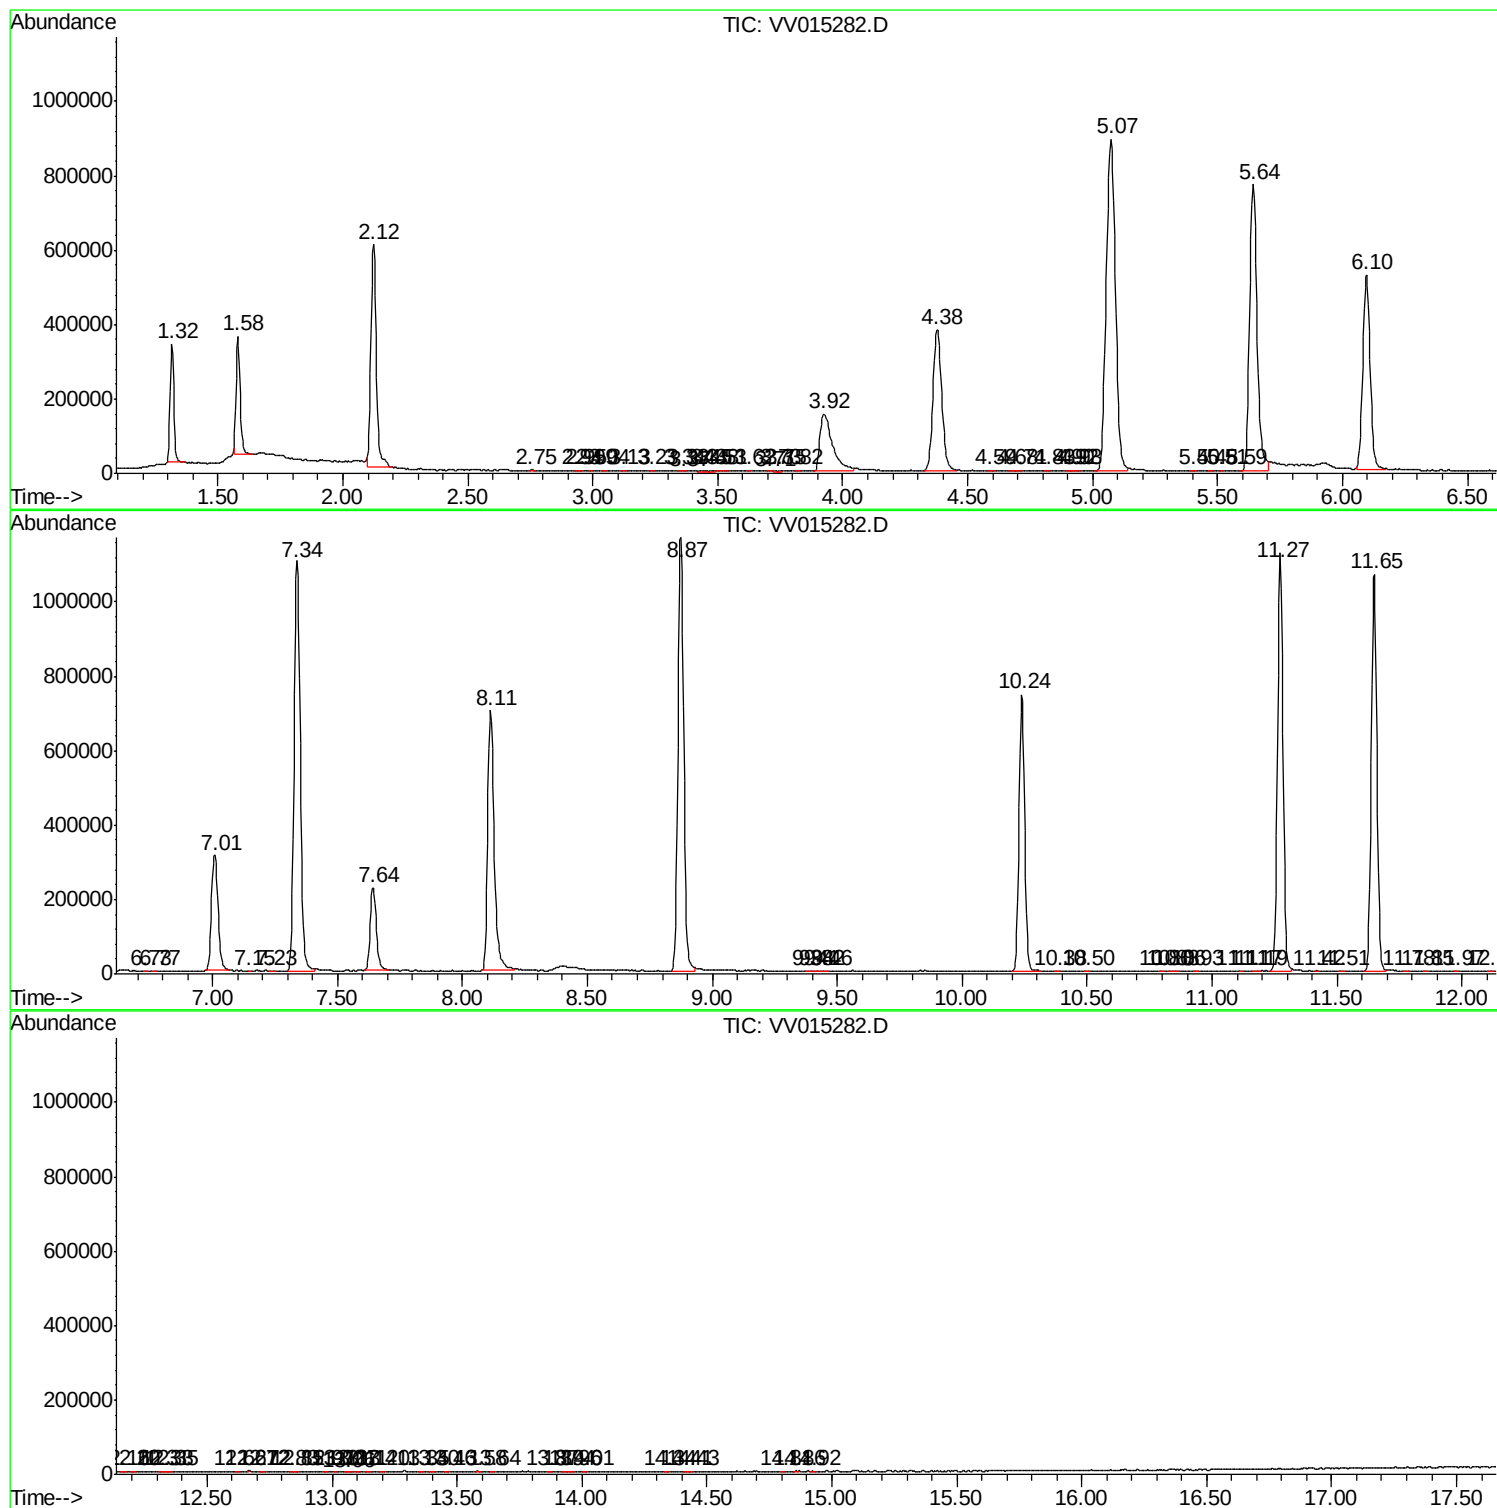

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015282.D
Acq On : 30 Mar 2020 19:19
Operator : SY/MD
Sample : VIBLK81
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK81

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015282.D
Acq On : 30 Mar 2020 19:19
Operator : SY/MD
Sample : VIBLK81
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK81

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc