

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015286.D
 Acq On : 30 Mar 2020 20:56
 Operator : SY/MD
 Sample : VIBLK83
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	351322	364238	15.55%	1.944%
2	1.579	146	152	166	rBV	316774	376456	16.07%	2.009%
3	2.122	313	321	354	rVB	669945	1029214	43.95%	5.492%
4	2.859	547	550	554	rBV6	1795	1359	0.06%	0.007%
5	2.904	562	564	567	rBV4	1750	894	0.04%	0.005%
6	2.929	570	572	575	rVB4	1584	732	0.03%	0.004%
7	3.042	602	607	610	rBV6	1467	1186	0.05%	0.006%
8	3.113	627	629	632	rBV3	1373	883	0.04%	0.005%
9	3.190	649	653	657	rBV6	1303	1206	0.05%	0.006%
10	3.360	703	706	708	rVB3	1579	750	0.03%	0.004%
11	3.524	752	757	761	rBV7	2191	2093	0.09%	0.011%
12	3.563	767	769	770	rBV2	1463	732	0.03%	0.004%
13	3.637	788	792	794	rBV4	1986	1134	0.05%	0.006%
14	3.662	797	800	803	rBV4	1045	935	0.04%	0.005%
15	3.733	818	822	825	rVB5	1434	975	0.04%	0.005%
16	3.759	825	830	833	rBV7	1664	1471	0.06%	0.008%
17	3.926	871	882	912	rBV2	144485	497719	21.25%	2.656%
18	4.379	1008	1023	1046	rVB	384658	936682	39.99%	4.998%
19	4.614	1094	1096	1099	rVB4	2276	913	0.04%	0.005%
20	4.679	1112	1116	1117	rBV4	1406	769	0.03%	0.004%
21	4.756	1137	1140	1144	rBV5	1486	1432	0.06%	0.008%
22	4.868	1173	1175	1178	rBV3	1407	932	0.04%	0.005%
23	4.939	1191	1197	1199	rVB7	1633	1414	0.06%	0.008%
24	4.981	1207	1210	1212	rBV3	1700	1071	0.05%	0.006%
25	5.006	1216	1218	1220	rBV3	1518	734	0.03%	0.004%
26	5.074	1222	1239	1266	rVV2	937221	2342009	100.00%	12.497%
27	5.344	1319	1323	1326	rBV6	1547	1120	0.05%	0.006%
28	5.392	1334	1338	1339	rBV2	1235	870	0.04%	0.005%
29	5.576	1392	1395	1397	rBV3	2711	1477	0.06%	0.008%
30	5.643	1401	1416	1437	rBV	717324	1440387	61.50%	7.686%
31	6.096	1544	1557	1577	rBV	531252	1059253	45.23%	5.652%
32	6.325	1626	1628	1630	rBV3	2021	935	0.04%	0.005%
33	6.383	1644	1646	1647	rBV2	1706	741	0.03%	0.004%
34	6.473	1672	1674	1677	rBV3	1523	863	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015286.D
 Acq On : 30 Mar 2020 20:56
 Operator : SY/MD
 Sample : VIBLK83
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	6.621	1715	1720	1722	rBV5	2467	2289	0.10%	0.012%
36	6.797	1772	1775	1777	rBV4	1269	917	0.04%	0.005%
37	6.894	1803	1805	1808	rBV4	1826	1281	0.05%	0.007%
38	7.010	1830	1841	1865	rVB	316829	569104	24.30%	3.037%
39	7.219	1901	1906	1909	rBV6	2573	2468	0.11%	0.013%
40	7.338	1931	1943	1966	rBV	1165009	1981966	84.63%	10.576%
41	7.643	2028	2038	2054	rBV	226074	379203	16.19%	2.023%
42	7.942	2129	2131	2133	rBV3	1505	787	0.03%	0.004%
43	8.042	2160	2162	2164	rBV2	2161	1244	0.05%	0.007%
44	8.112	2174	2184	2213	rBV	668898	1243644	53.10%	6.636%
45	8.813	2399	2402	2404	rBV4	2053	1408	0.06%	0.008%
46	8.874	2409	2421	2440	rBV	1137418	1819963	77.71%	9.712%
47	9.331	2561	2563	2566	rVB4	1605	876	0.04%	0.005%
48	9.379	2576	2578	2582	rVB5	1159	701	0.03%	0.004%
49	9.440	2594	2597	2601	rBV6	2246	2071	0.09%	0.011%
50	9.473	2604	2607	2610	rBV4	3208	1964	0.08%	0.010%
51	9.514	2618	2620	2626	rVB6	1621	1286	0.05%	0.007%
52	9.736	2686	2689	2691	rBV4	1855	1105	0.05%	0.006%
53	9.784	2701	2704	2705	rBV2	1425	813	0.03%	0.004%
54	9.839	2718	2721	2727	rVB7	2405	2404	0.10%	0.013%
55	9.926	2743	2748	2751	rBV7	2522	2334	0.10%	0.012%
56	9.997	2768	2770	2773	rBV3	1579	1105	0.05%	0.006%
57	10.180	2824	2827	2830	rBV3	2279	1561	0.07%	0.008%
58	10.238	2834	2845	2865	rVB	726348	1149036	49.06%	6.131%
59	10.518	2930	2932	2936	rBV5	1121	854	0.04%	0.005%
60	10.540	2936	2939	2941	rBV3	1933	1165	0.05%	0.006%
61	10.733	2996	2999	3002	rBV5	1422	1030	0.04%	0.005%
62	10.794	3015	3018	3020	rBV3	2357	1797	0.08%	0.010%
63	10.845	3032	3034	3038	rVB5	1969	1106	0.05%	0.006%
64	10.871	3038	3042	3043	rBV4	2040	1284	0.05%	0.007%
65	10.935	3058	3062	3064	rBV4	2161	1578	0.07%	0.008%
66	10.993	3075	3080	3081	rBV5	2338	1905	0.08%	0.010%
67	11.035	3091	3093	3095	rVB3	1718	757	0.03%	0.004%
68	11.151	3126	3129	3136	rVB9	2356	2742	0.12%	0.015%
69	11.190	3136	3141	3143	rBV5	3146	3149	0.13%	0.017%
70	11.273	3154	3167	3185	rBV	1092289	1690993	72.20%	9.023%
71	11.517	3239	3243	3246	rBV5	1903	1899	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015286.D
 Acq On : 30 Mar 2020 20:56
 Operator : SY/MD
 Sample : VIBLK83
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.649	3272	3284	3301	rBV	1128970	1745761	74.54%	9.316%
73	11.788	3325	3327	3329	rBV3	1829	1067	0.05%	0.006%
74	11.807	3331	3333	3335	rVB3	2523	1024	0.04%	0.005%
75	11.871	3349	3353	3354	rBV3	2162	1053	0.04%	0.006%
76	11.910	3361	3365	3368	rBV5	1600	1461	0.06%	0.008%
77	12.022	3397	3400	3401	rBV3	1599	868	0.04%	0.005%
78	12.077	3415	3417	3420	rBV3	1428	863	0.04%	0.005%
79	12.161	3441	3443	3445	rBV3	1303	763	0.03%	0.004%
80	12.170	3445	3446	3449	rVV3	1203	712	0.03%	0.004%
81	12.206	3455	3457	3463	rVB6	2081	1398	0.06%	0.007%
82	12.440	3523	3530	3534	rBV10	2325	3112	0.13%	0.017%
83	12.662	3596	3599	3601	rBV4	1710	1217	0.05%	0.006%
84	12.736	3618	3622	3624	rBV5	2037	1351	0.06%	0.007%
85	12.768	3627	3632	3636	rVB7	2060	1923	0.08%	0.010%
86	12.791	3636	3639	3641	rBV3	1843	878	0.04%	0.005%
87	12.871	3661	3664	3666	rBV4	1677	1073	0.05%	0.006%
88	13.035	3712	3715	3717	rBV3	1500	884	0.04%	0.005%
89	13.154	3750	3752	3755	rBV3	1470	826	0.04%	0.004%
90	13.189	3761	3763	3767	rBV4	1716	1302	0.06%	0.007%
91	13.276	3788	3790	3792	rBV3	1802	983	0.04%	0.005%
92	13.331	3804	3807	3810	rBV5	2925	2010	0.09%	0.011%
93	13.469	3848	3850	3853	rBV4	1630	1002	0.04%	0.005%
94	13.726	3927	3930	3932	rBV4	2925	2154	0.09%	0.011%
95	14.096	4041	4045	4050	rBV8	2075	2363	0.10%	0.013%
96	14.199	4075	4077	4079	rBV2	1899	986	0.04%	0.005%
97	14.247	4088	4092	4098	rVB7	3811	4182	0.18%	0.022%
98	14.276	4098	4101	4106	rBV6	2197	2488	0.11%	0.013%
99	14.382	4131	4134	4138	rVB5	2528	1509	0.06%	0.008%
100	15.157	4372	4375	4377	rBV4	2145	1548	0.07%	0.008%


Sum of corrected areas: 18740129

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015286.D
Acq On : 30 Mar 2020 20:56
Operator : SY/MD
Sample : VIBLK83
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

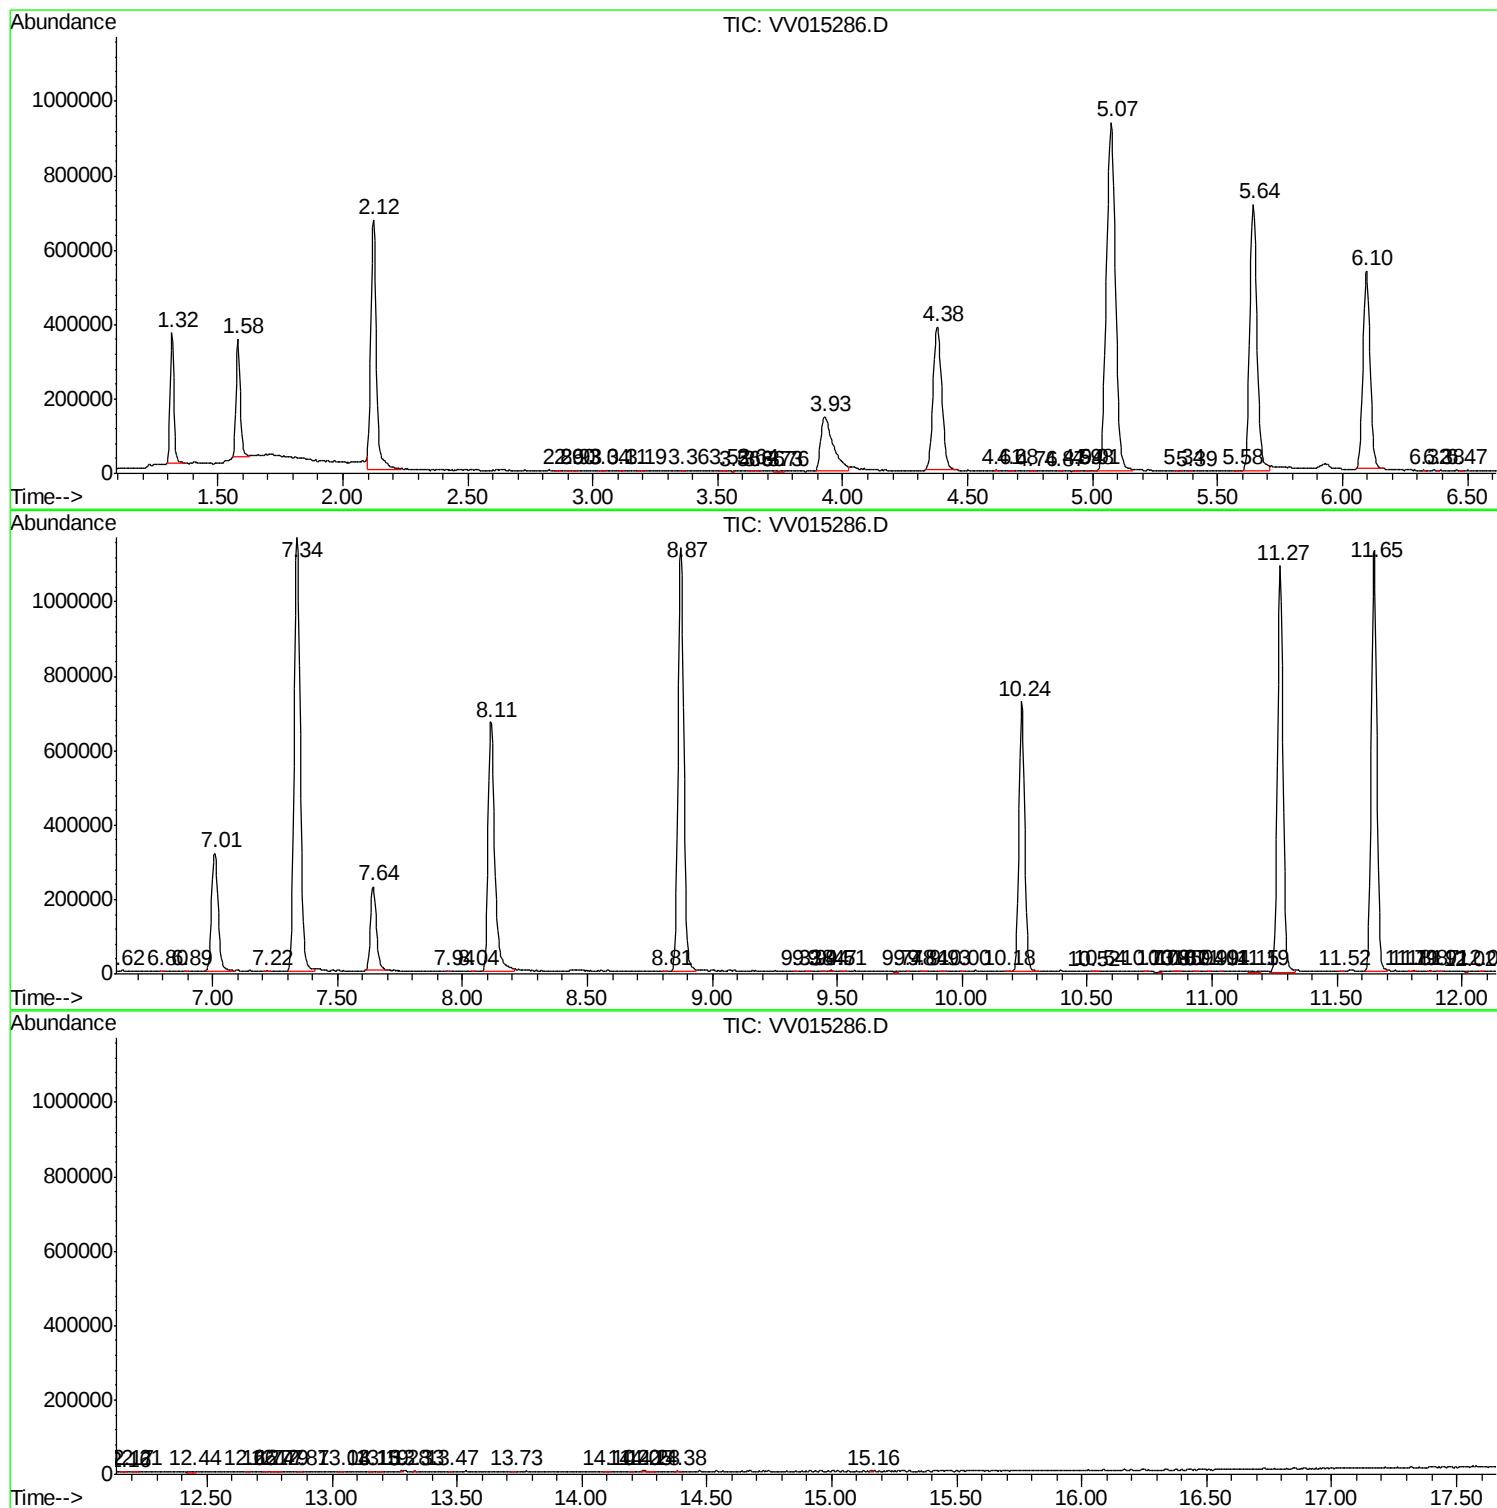

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015286.D
Acq On : 30 Mar 2020 20:56
Operator : SY/MD
Sample : VIBLK83
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033020\
Data File : VV015286.D
Acq On : 30 Mar 2020 20:56
Operator : SY/MD
Sample : VIBLK83
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc