

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015288.D
 Acq On : 30 Mar 2020 21:44
 Operator : SY/MD
 Sample : VIBLK84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	337459	345420	15.26%	1.852%
2	1.579	147	152	166	rVB	309489	360492	15.93%	1.933%
3	2.122	313	321	346	rVB	628615	959933	42.42%	5.147%
4	2.701	498	501	504	rBV5	1913	1622	0.07%	0.009%
5	2.949	576	578	579	rBV2	1631	746	0.03%	0.004%
6	3.055	607	611	613	rBV4	1779	1090	0.05%	0.006%
7	3.068	613	615	617	rVV3	1638	640	0.03%	0.003%
8	3.158	642	643	645	rBV2	1378	613	0.03%	0.003%
9	3.222	660	663	664	rBV3	1792	1145	0.05%	0.006%
10	3.277	678	680	683	rVB4	1571	664	0.03%	0.004%
11	3.322	690	694	699	rBV7	3048	3311	0.15%	0.018%
12	3.354	700	704	707	rVB4	2674	1924	0.09%	0.010%
13	3.380	707	712	713	rBV5	2124	1774	0.08%	0.010%
14	3.408	718	721	724	rBV5	1964	1678	0.07%	0.009%
15	3.447	731	733	736	rVB4	2658	1372	0.06%	0.007%
16	3.511	748	753	757	rBV6	1902	1891	0.08%	0.010%
17	3.534	757	760	762	rBV4	1280	670	0.03%	0.004%
18	3.553	762	766	769	rBV5	1632	1262	0.06%	0.007%
19	3.621	783	787	790	rBV6	1861	1268	0.06%	0.007%
20	3.714	815	816	818	rVB3	909	253	0.01%	0.001%
21	3.836	850	854	859	rBV7	2221	2233	0.10%	0.012%
22	3.926	870	882	921	rBV2	144917	525694	23.23%	2.819%
23	4.376	1009	1022	1045	rVB2	368096	895943	39.59%	4.804%
24	4.749	1133	1138	1141	rBV6	1917	1834	0.08%	0.010%
25	4.801	1147	1154	1160	rVB9	1660	1972	0.09%	0.011%
26	4.881	1177	1179	1182	rBV4	1666	1469	0.06%	0.008%
27	4.939	1194	1197	1199	rVB4	1406	749	0.03%	0.004%
28	4.981	1208	1210	1211	rBV2	1053	344	0.02%	0.002%
29	5.010	1218	1219	1220	rBV	1222	352	0.02%	0.002%
30	5.074	1220	1239	1262	rVV2	889028	2263047	100.00%	12.135%
31	5.479	1362	1365	1367	rBV4	1530	889	0.04%	0.005%
32	5.585	1393	1398	1401	rBV6	2916	2595	0.11%	0.014%
33	5.643	1403	1416	1437	rBV	774894	1600763	70.73%	8.583%
34	6.093	1545	1556	1580	rVB	519576	1040304	45.97%	5.578%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015288.D
 Acq On : 30 Mar 2020 21:44
 Operator : SY/MD
 Sample : VIBLK84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	6.424	1656	1659	1661	rBV3	2109	1302	0.06%	0.007%
36	6.572	1703	1705	1707	rBV3	1182	385	0.02%	0.002%
37	6.730	1751	1754	1758	rBV4	1872	1508	0.07%	0.008%
38	7.006	1831	1840	1859	rVB	314685	547803	24.21%	2.937%
39	7.338	1931	1943	1964	rBV	1123126	1926863	85.14%	10.332%
40	7.643	2029	2038	2056	rVB	217442	367399	16.23%	1.970%
41	8.112	2174	2184	2213	rBV	665363	1234748	54.56%	6.621%
42	8.765	2384	2387	2390	rBV5	2249	1189	0.05%	0.006%
43	8.874	2409	2421	2441	rBV	1172279	1898428	83.89%	10.180%
44	9.376	2575	2577	2579	rVB4	1908	792	0.03%	0.004%
45	9.482	2608	2610	2612	rBV3	1839	1212	0.05%	0.006%
46	10.154	2817	2819	2820	rBV2	1267	339	0.01%	0.002%
47	10.238	2832	2845	2868	rBV	714562	1131224	49.99%	6.066%
48	10.505	2926	2928	2932	rVB5	1432	687	0.03%	0.004%
49	10.662	2974	2977	2978	rBV3	1406	826	0.04%	0.004%
50	10.746	3001	3003	3006	rBV3	1619	1009	0.04%	0.005%
51	10.804	3019	3021	3028	rVB8	1495	1143	0.05%	0.006%
52	10.916	3052	3056	3059	rVB6	2593	2045	0.09%	0.011%
53	10.935	3059	3062	3063	rBV3	2534	1545	0.07%	0.008%
54	10.971	3071	3073	3074	rBV2	1586	622	0.03%	0.003%
55	11.000	3078	3082	3085	rBV5	1598	1650	0.07%	0.009%
56	11.029	3090	3091	3093	rBV2	740	390	0.02%	0.002%
57	11.119	3116	3119	3124	rBV7	1803	1399	0.06%	0.008%
58	11.144	3124	3127	3128	rBV2	922	466	0.02%	0.002%
59	11.273	3155	3167	3185	rBV	1156558	1774350	78.41%	9.514%
60	11.649	3272	3284	3301	rBV	1089026	1686529	74.52%	9.043%
61	11.871	3351	3353	3355	rVB3	1322	472	0.02%	0.003%
62	11.906	3362	3364	3365	rBV2	1047	342	0.02%	0.002%
63	12.022	3398	3400	3402	rBV2	982	457	0.02%	0.002%
64	12.038	3402	3405	3406	rBV3	1852	933	0.04%	0.005%
65	12.096	3420	3423	3425	rBV4	1382	965	0.04%	0.005%
66	12.125	3430	3432	3433	rBV2	532	199	0.01%	0.001%
67	12.135	3433	3435	3436	rBV2	1622	696	0.03%	0.004%
68	12.206	3454	3457	3461	rBV4	1477	1246	0.06%	0.007%
69	12.251	3468	3471	3473	rBV3	1846	1482	0.07%	0.008%
70	12.373	3503	3509	3511	rBV7	2912	2727	0.12%	0.015%
71	12.501	3548	3549	3553	rVB4	1318	762	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015288.D
 Acq On : 30 Mar 2020 21:44
 Operator : SY/MD
 Sample : VIBLK84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	12.569	3565	3570	3572	rBV4	1596	1513	0.07%	0.008%
73	12.627	3585	3588	3590	rBV4	1446	953	0.04%	0.005%
74	12.672	3600	3602	3605	rBV3	2241	1366	0.06%	0.007%
75	12.726	3614	3619	3621	rBV5	1423	1293	0.06%	0.007%
76	12.752	3625	3627	3630	rBV2	1212	743	0.03%	0.004%
77	12.813	3644	3646	3647	rBV2	815	369	0.02%	0.002%
78	12.858	3658	3660	3665	rVB6	2898	1864	0.08%	0.010%
79	12.881	3665	3667	3668	rVB2	692	229	0.01%	0.001%
80	12.897	3668	3672	3673	rBV3	1856	1279	0.06%	0.007%
81	13.067	3722	3725	3727	rVB4	1604	904	0.04%	0.005%
82	13.443	3840	3842	3843	rBV2	1181	409	0.02%	0.002%
83	13.498	3855	3859	3862	rBV6	1542	1501	0.07%	0.008%
84	13.582	3882	3885	3889	rVB6	2282	1496	0.07%	0.008%
85	13.604	3889	3892	3894	rBV4	2621	1607	0.07%	0.009%
86	13.697	3917	3921	3925	rBV6	1878	1839	0.08%	0.010%
87	13.855	3968	3970	3971	rBV	1848	823	0.04%	0.004%
88	13.890	3979	3981	3986	rVB6	1580	1160	0.05%	0.006%
89	14.012	4017	4019	4023	rBV4	2237	1316	0.06%	0.007%
90	14.148	4059	4061	4065	rVB5	1699	941	0.04%	0.005%
91	14.948	4303	4310	4311	rBV5	2997	3023	0.13%	0.016%
92	15.144	4367	4371	4373	rBV4	3573	2693	0.12%	0.014%


Sum of corrected areas: 18649411

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015288.D
Acq On : 30 Mar 2020 21:44
Operator : SY/MD
Sample : VIBLK84
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK84

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

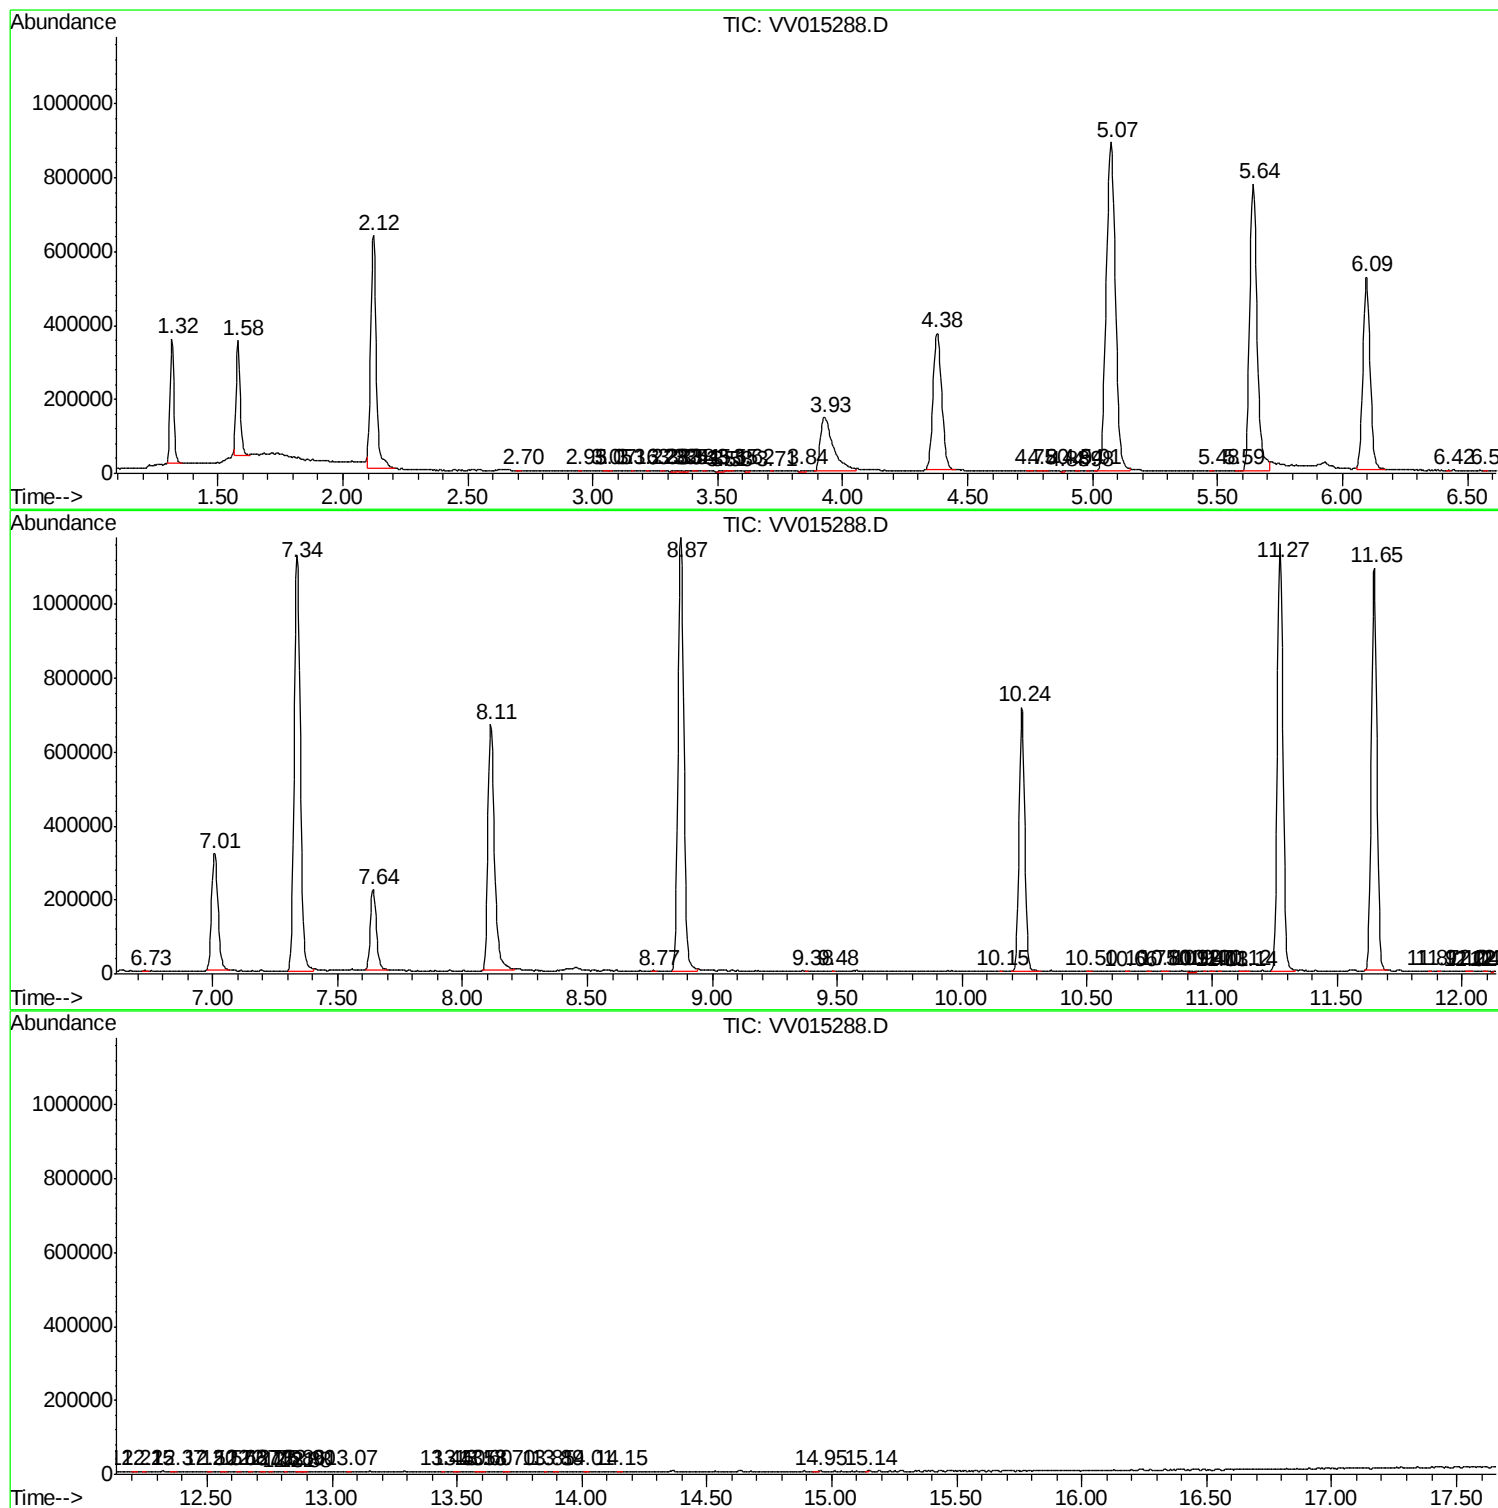

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015288.D
Acq On : 30 Mar 2020 21:44
Operator : SY/MD
Sample : VIBLK84
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK84

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033020\
Data File : VV015288.D
Acq On : 30 Mar 2020 21:44
Operator : SY/MD
Sample : VIBLK84
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK84

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc