

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015290.D
 Acq On : 30 Mar 2020 22:32
 Operator : SY/MD
 Sample : L1976-21DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	343674	355172	15.32%	1.775%
2	1.579	146	152	166	rBV	307932	373603	16.12%	1.867%
3	2.122	313	321	342	rVB	647303	957997	41.33%	4.788%
4	2.756	514	518	519	rBV3	1491	896	0.04%	0.004%
5	2.920	566	569	570	rBV3	1110	636	0.03%	0.003%
6	2.955	577	580	582	rBV4	2175	1251	0.05%	0.006%
7	3.036	603	605	606	rBV2	1427	674	0.03%	0.003%
8	3.061	611	613	616	rBV3	1516	1057	0.05%	0.005%
9	3.110	624	628	630	rBV5	2091	1718	0.07%	0.009%
10	3.171	642	647	650	rBV7	1834	1713	0.07%	0.009%
11	3.212	658	660	663	rBV3	1132	599	0.03%	0.003%
12	3.267	675	677	681	rBV5	1467	1025	0.04%	0.005%
13	3.341	697	700	702	rBV3	1870	1001	0.04%	0.005%
14	3.389	713	715	717	rVB3	1841	845	0.04%	0.004%
15	3.476	739	742	743	rBV3	1052	621	0.03%	0.003%
16	3.508	749	752	753	rBV3	1500	722	0.03%	0.004%
17	3.608	779	783	790	rBV10	2539	3440	0.15%	0.017%
18	3.650	790	796	798	rVV7	1594	1395	0.06%	0.007%
19	3.736	819	823	825	rBV4	1345	1057	0.05%	0.005%
20	3.749	825	827	830	rVB4	1526	787	0.03%	0.004%
21	3.810	844	846	848	rBV2	1244	611	0.03%	0.003%
22	3.875	864	866	869	rBV4	1651	831	0.04%	0.004%
23	3.933	871	884	918	rBV2	141368	546987	23.60%	2.734%
24	4.380	1007	1023	1051	rBV	378904	925551	39.93%	4.626%
25	4.682	1114	1117	1119	rBV4	1337	916	0.04%	0.005%
26	4.743	1131	1136	1138	rBV5	2270	2355	0.10%	0.012%
27	4.772	1143	1145	1151	rVV6	1523	1376	0.06%	0.007%
28	4.810	1155	1157	1159	rBV3	1798	888	0.04%	0.004%
29	4.939	1194	1197	1199	rBV4	1666	1074	0.05%	0.005%
30	5.074	1217	1239	1268	rBV2	919079	2318125	100.00%	11.586%
31	5.363	1326	1329	1333	rVB5	2260	1751	0.08%	0.009%
32	5.386	1333	1336	1339	rBV5	1752	1639	0.07%	0.008%
33	5.495	1367	1370	1372	rBV4	2775	1794	0.08%	0.009%
34	5.643	1403	1416	1434	rBV	716690	1409377	60.80%	7.044%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015290.D
 Acq On : 30 Mar 2020 22:32
 Operator : SY/MD
 Sample : L1976-21DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	5.939	1496	1508	1527	rVB	765879	1466205	63.25%	7.328%
36	6.097	1545	1557	1586	rVB	520301	10555871	45.55%	5.277%
37	6.617	1712	1719	1720	rBV7	2728	3002	0.13%	0.015%
38	6.752	1758	1761	1764	rBV4	1983	1272	0.05%	0.006%
39	6.769	1764	1766	1769	rBV4	2014	1279	0.06%	0.006%
40	7.010	1823	1841	1864	rBV	316907	575388	24.82%	2.876%
41	7.338	1931	1943	1962	rBV	1132402	1942741	83.81%	9.710%
42	7.643	2027	2038	2054	rBV	227231	384325	16.58%	1.921%
43	7.945	2129	2132	2135	rVB4	2979	1246	0.05%	0.006%
44	7.994	2144	2147	2150	rBV3	2827	2239	0.10%	0.011%
45	8.045	2161	2163	2167	rBV3	1663	884	0.04%	0.004%
46	8.116	2173	2185	2212	rBV	650263	1237314	53.38%	6.184%
47	8.785	2391	2393	2396	rVB4	1678	962	0.04%	0.005%
48	8.804	2397	2399	2401	rBV2	2224	881	0.04%	0.004%
49	8.875	2410	2421	2438	rBV	1126203	1802621	77.76%	9.010%
50	9.347	2566	2568	2574	rBV6	2196	1958	0.08%	0.010%
51	9.447	2597	2599	2601	rVB2	1975	825	0.04%	0.004%
52	9.521	2620	2622	2625	rBV4	1229	791	0.03%	0.004%
53	9.559	2629	2634	2635	rBV3	2100	1728	0.07%	0.009%
54	9.662	2664	2666	2669	rBV4	1326	927	0.04%	0.005%
55	9.727	2683	2686	2687	rBV3	979	619	0.03%	0.003%
56	9.794	2703	2707	2708	rBV3	3122	1808	0.08%	0.009%
57	9.955	2755	2757	2759	rBV3	1304	791	0.03%	0.004%
58	10.003	2769	2772	2774	rBV3	2016	1038	0.04%	0.005%
59	10.112	2804	2806	2810	rVB4	1205	683	0.03%	0.003%
60	10.135	2811	2813	2816	rVV4	1512	762	0.03%	0.004%
61	10.170	2822	2824	2826	rBV3	1477	770	0.03%	0.004%
62	10.238	2829	2845	2863	rBV	735222	1144406	49.37%	5.720%
63	10.492	2922	2924	2926	rBV3	1255	560	0.02%	0.003%
64	10.659	2974	2976	2980	rBV4	2138	1215	0.05%	0.006%
65	10.752	3003	3005	3007	rBV3	2152	1183	0.05%	0.006%
66	10.804	3014	3021	3025	rBV9	2228	2701	0.12%	0.013%
67	11.273	3154	3167	3187	rBV	1117187	1693077	73.04%	8.462%
68	11.450	3219	3222	3227	rBV6	1911	1822	0.08%	0.009%
69	11.540	3247	3250	3253	rBV5	2554	2054	0.09%	0.010%
70	11.646	3272	3283	3301	rBV	1095457	1714545	73.96%	8.570%
71	11.823	3336	3338	3341	rBV4	1505	899	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015290.D
 Acq On : 30 Mar 2020 22:32
 Operator : SY/MD
 Sample : L1976-21DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.935	3370	3373	3376	rBV4	1702	1333	0.06%	0.007%
73	11.984	3384	3388	3389	rBV4	1836	1263	0.05%	0.006%
74	12.112	3425	3428	3429	rBV3	1442	672	0.03%	0.003%
75	12.141	3434	3437	3439	rBV3	1923	1350	0.06%	0.007%
76	12.186	3449	3451	3455	rBV5	1223	1042	0.04%	0.005%
77	12.235	3462	3466	3469	rBV6	1510	1686	0.07%	0.008%
78	12.415	3519	3522	3525	rBV4	2338	1535	0.07%	0.008%
79	12.460	3534	3536	3539	rBV2	1292	973	0.04%	0.005%
80	12.563	3566	3568	3571	rBV4	1780	1072	0.05%	0.005%
81	12.659	3590	3598	3602	rBV10	2144	3118	0.13%	0.016%
82	12.701	3609	3611	3613	rVB3	1305	535	0.02%	0.003%
83	12.720	3613	3617	3620	rBV4	1820	1461	0.06%	0.007%
84	12.778	3633	3635	3638	rBV3	1231	612	0.03%	0.003%
85	12.800	3638	3642	3644	rBV4	1327	941	0.04%	0.005%
86	12.977	3695	3697	3700	rBV3	1561	922	0.04%	0.005%
87	13.009	3705	3707	3709	rBV3	1796	773	0.03%	0.004%
88	13.135	3744	3746	3748	rVB2	1321	549	0.02%	0.003%
89	13.151	3748	3751	3752	rBV3	1324	743	0.03%	0.004%
90	13.234	3774	3777	3779	rBV4	1880	1375	0.06%	0.007%
91	13.370	3814	3819	3823	rBV8	2422	2745	0.12%	0.014%
92	13.427	3832	3837	3838	rBV4	1703	1515	0.07%	0.008%
93	13.460	3844	3847	3849	rBV4	1137	778	0.03%	0.004%
94	13.524	3864	3867	3869	rBV3	1679	1149	0.05%	0.006%
95	13.633	3899	3901	3904	rVB4	1478	784	0.03%	0.004%
96	13.868	3971	3974	3976	rBV3	1276	834	0.04%	0.004%
97	14.492	4164	4168	4169	rBV3	2307	1853	0.08%	0.009%
98	14.533	4178	4181	4183	rBV4	2107	1596	0.07%	0.008%
99	14.649	4213	4217	4219	rBV4	2976	2061	0.09%	0.010%
100	14.691	4228	4230	4233	rBV4	1946	1315	0.06%	0.007%


Sum of corrected areas: 20007461

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015290.D
Acq On : 30 Mar 2020 22:32
Operator : SY/MD
Sample : L1976-21DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

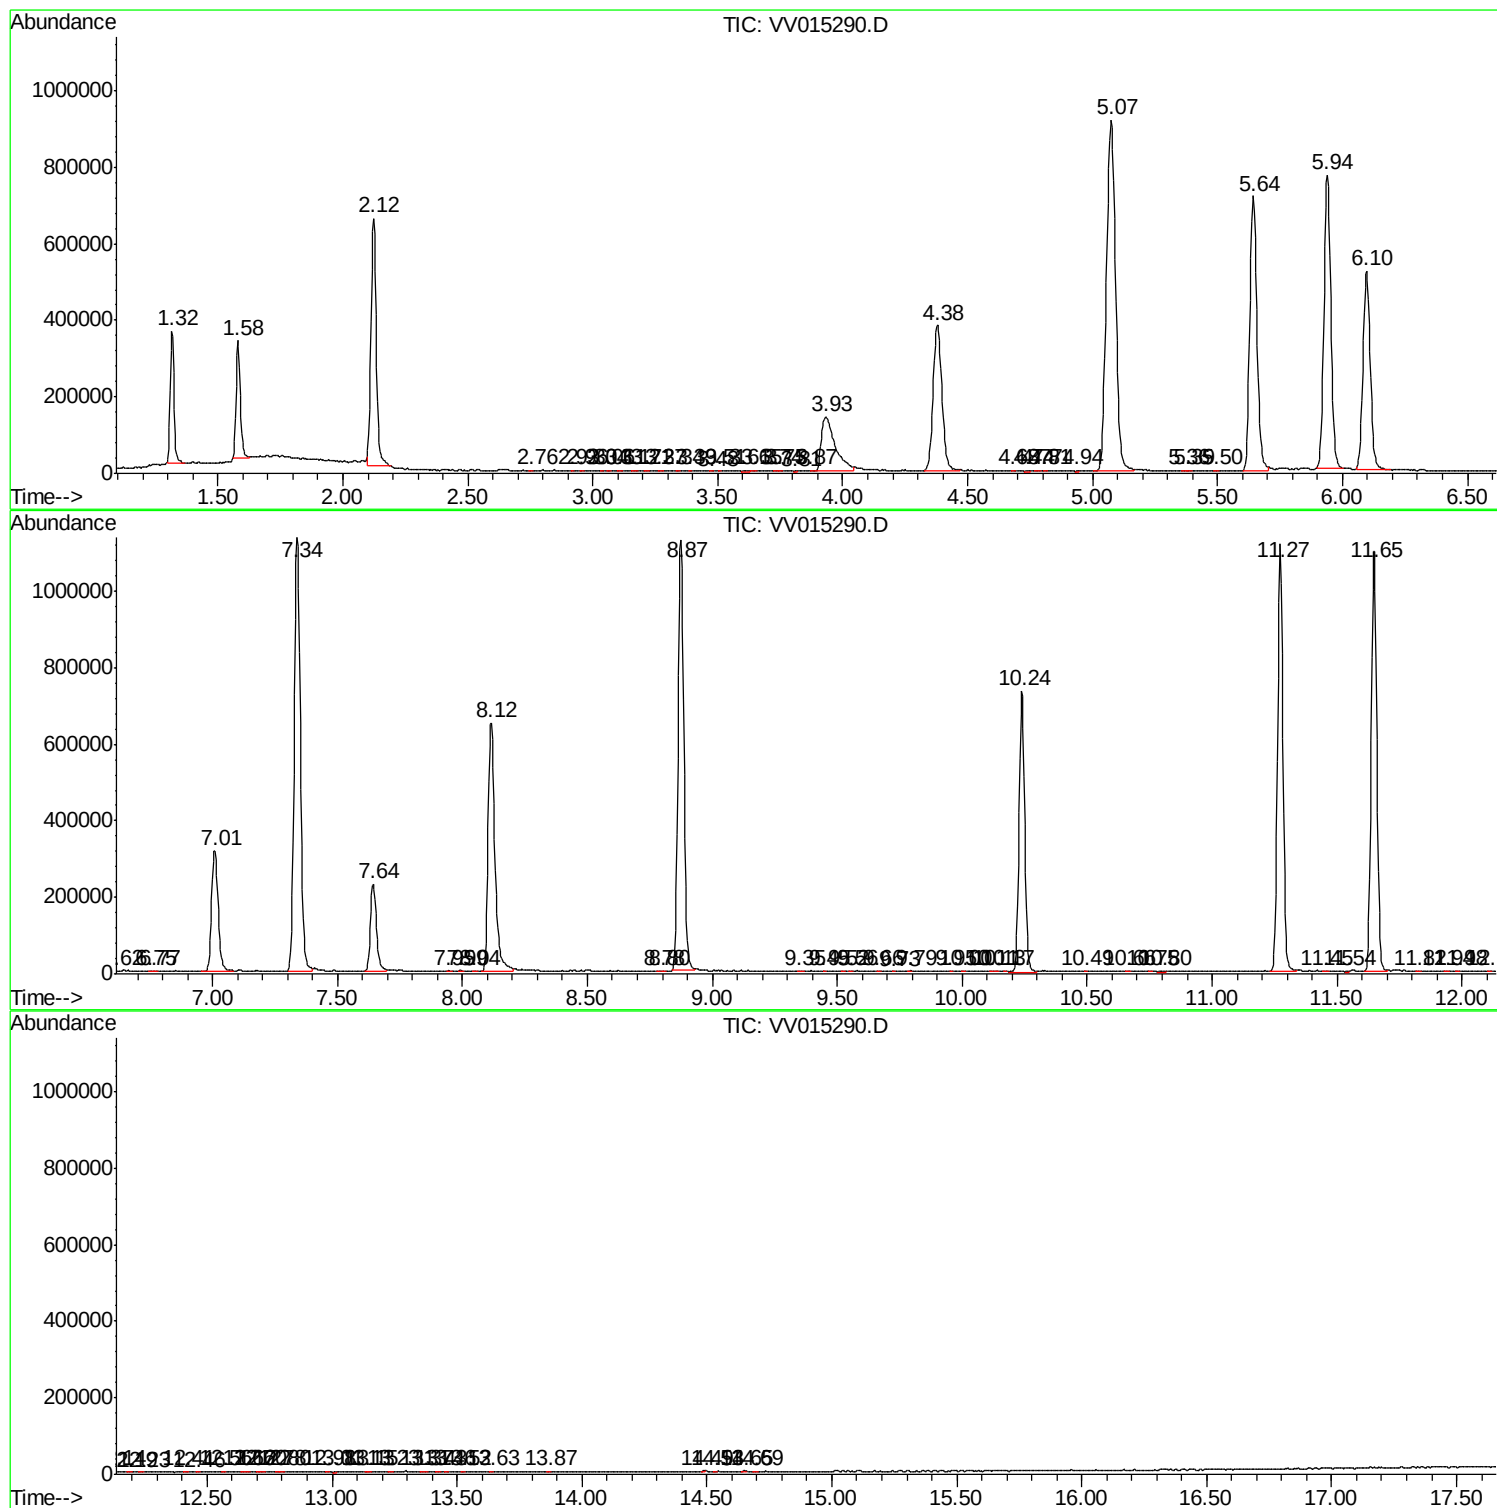

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015290.D
Acq On : 30 Mar 2020 22:32
Operator : SY/MD
Sample : L1976-21DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033020\
Data File : VV015290.D
Acq On : 30 Mar 2020 22:32
Operator : SY/MD
Sample : L1976-21DL 5X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTK6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc