

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015292.D
 Acq On : 30 Mar 2020 23:21
 Operator : SY/MD
 Sample : L1976-06 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTLO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	88	rVB2	1191091	1306197	53.91%	6.408%
2	1.579	146	152	165	rBV	294761	354708	14.64%	1.740%
3	2.116	311	319	334	rVB	675847	951618	39.28%	4.668%
4	3.177	641	649	653	rBV10	2380	3498	0.14%	0.017%
5	3.290	682	684	686	rBV2	1014	535	0.02%	0.003%
6	3.322	692	694	695	rBV2	1313	579	0.02%	0.003%
7	3.354	702	704	707	rBV3	1266	737	0.03%	0.004%
8	3.444	728	732	733	rBV4	997	503	0.02%	0.002%
9	3.489	743	746	750	rVB6	2264	1363	0.06%	0.007%
10	3.569	769	771	776	rBV4	1690	1116	0.05%	0.005%
11	3.647	793	795	798	rVB4	1079	494	0.02%	0.002%
12	3.692	805	809	810	rBV4	1434	1039	0.04%	0.005%
13	3.782	835	837	843	rVB7	1704	1218	0.05%	0.006%
14	3.939	871	886	924	rBV2	160002	622368	25.69%	3.053%
15	4.376	1008	1022	1046	rVB	389449	956981	39.50%	4.695%
16	4.540	1071	1073	1076	rVB4	1923	1132	0.05%	0.006%
17	4.592	1087	1089	1091	rBV3	1093	496	0.02%	0.002%
18	4.772	1143	1145	1147	rBV3	1273	769	0.03%	0.004%
19	4.878	1176	1178	1182	rBV4	1219	967	0.04%	0.005%
20	4.913	1186	1189	1195	rVB8	1565	1333	0.06%	0.007%
21	4.962	1201	1204	1209	rBV6	1147	1300	0.05%	0.006%
22	5.071	1221	1238	1259	rBV2	977829	2422849	100.00%	11.886%
23	5.299	1306	1309	1310	rBV2	1341	765	0.03%	0.004%
24	5.495	1368	1370	1371	rBV2	2515	1150	0.05%	0.006%
25	5.640	1402	1415	1438	rBV	737474	1456855	60.13%	7.147%
26	6.093	1544	1556	1580	rVB	547400	1106640	45.68%	5.429%
27	6.627	1715	1722	1723	rBV7	2095	2186	0.09%	0.011%
28	6.788	1769	1772	1777	rVB7	2117	1985	0.08%	0.010%
29	6.872	1796	1798	1802	rBV5	2393	1792	0.07%	0.009%
30	6.942	1817	1820	1822	rBV3	1882	1368	0.06%	0.007%
31	7.007	1830	1840	1859	rBV	333112	589521	24.33%	2.892%
32	7.148	1882	1884	1886	rBV3	1595	850	0.04%	0.004%
33	7.338	1931	1943	1962	rBV	1187139	2023076	83.50%	9.925%
34	7.643	2028	2038	2055	rBV	233780	404092	16.68%	1.982%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015292.D
 Acq On : 30 Mar 2020 23:21
 Operator : SY/MD
 Sample : L1976-06 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTLO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	7.939	2127	2130	2133	rBV5	1970	1047	0.04%	0.005%
36	7.997	2141	2148	2158	rVB5	5017	9767	0.40%	0.048%
37	8.035	2158	2160	2167	rVB6	2201	2022	0.08%	0.010%
38	8.119	2171	2186	2214	rBV	630818	1327497	54.79%	6.512%
39	8.383	2263	2268	2271	rBV6	3348	2999	0.12%	0.015%
40	8.418	2275	2279	2280	rBV4	2002	1480	0.06%	0.007%
41	8.508	2304	2307	2309	rBV4	1899	1416	0.06%	0.007%
42	8.875	2405	2421	2442	rBV	1139968	1881616	77.66%	9.231%
43	9.370	2572	2575	2576	rBV2	1499	856	0.04%	0.004%
44	9.479	2607	2609	2613	rVB4	1419	841	0.03%	0.004%
45	9.569	2628	2637	2639	rBV2	14196	17347	0.72%	0.085%
46	9.633	2654	2657	2661	rVB6	2286	1951	0.08%	0.010%
47	9.659	2661	2665	2670	rBV6	1682	1774	0.07%	0.009%
48	9.723	2683	2685	2686	rBV2	1413	486	0.02%	0.002%
49	9.994	2767	2769	2772	rBV3	2064	899	0.04%	0.004%
50	10.045	2783	2785	2790	rVB5	1580	1142	0.05%	0.006%
51	10.068	2790	2792	2795	rVB3	2080	959	0.04%	0.005%
52	10.090	2795	2799	2802	rBV5	1657	1603	0.07%	0.008%
53	10.109	2802	2805	2807	rVB3	1459	847	0.03%	0.004%
54	10.177	2824	2826	2827	rBV2	1666	681	0.03%	0.003%
55	10.241	2832	2846	2863	rBV	770456	1236350	51.03%	6.065%
56	10.428	2903	2904	2906	rBV2	1267	578	0.02%	0.003%
57	10.633	2966	2968	2970	rVB3	1443	610	0.03%	0.003%
58	10.817	3023	3025	3030	rVB5	1721	1391	0.06%	0.007%
59	10.846	3030	3034	3036	rBV4	1646	1110	0.05%	0.005%
60	10.862	3036	3039	3041	rBV3	1880	1385	0.06%	0.007%
61	10.939	3053	3063	3075	rBV3	10490	20329	0.84%	0.100%
62	11.010	3083	3085	3088	rBV3	2095	1460	0.06%	0.007%
63	11.071	3100	3104	3105	rBV3	1588	1215	0.05%	0.006%
64	11.138	3122	3125	3127	rBV3	1468	916	0.04%	0.004%
65	11.273	3155	3167	3191	rBV	1148109	1751991	72.31%	8.595%
66	11.505	3236	3239	3240	rBV3	1702	1005	0.04%	0.005%
67	11.649	3272	3284	3304	rBV	1168024	1822657	75.23%	8.941%
68	12.067	3410	3414	3416	rBV4	1278	993	0.04%	0.005%
69	12.084	3416	3419	3421	rVB3	1222	907	0.04%	0.004%
70	12.180	3444	3449	3450	rBV5	1277	956	0.04%	0.005%
71	12.193	3450	3453	3456	rBV5	880	545	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015292.D
 Acq On : 30 Mar 2020 23:21
 Operator : SY/MD
 Sample : L1976-06 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTLO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	12.209	3456	3458	3460	rBV4	1305	741	0.03%	0.004%
73	12.235	3461	3466	3468	rVB6	1900	1538	0.06%	0.008%
74	12.251	3468	3471	3474	rBV5	1659	919	0.04%	0.005%
75	12.270	3474	3477	3479	rBV4	2350	1577	0.07%	0.008%
76	12.331	3494	3496	3501	rVB6	1543	978	0.04%	0.005%
77	12.440	3528	3530	3532	rBV3	1701	776	0.03%	0.004%
78	12.482	3542	3543	3546	rVB2	2314	833	0.03%	0.004%
79	12.502	3546	3549	3552	rBV4	1622	1272	0.05%	0.006%
80	12.534	3557	3559	3563	rVB5	1259	816	0.03%	0.004%
81	12.566	3566	3569	3572	rBV4	2232	1905	0.08%	0.009%
82	12.675	3597	3603	3608	rVB7	5097	6860	0.28%	0.034%
83	12.794	3636	3640	3642	rBV5	1355	1053	0.04%	0.005%
84	12.865	3660	3662	3663	rBV2	1364	541	0.02%	0.003%
85	12.936	3683	3684	3686	rBV2	2000	964	0.04%	0.005%
86	13.129	3741	3744	3747	rBV4	2636	1897	0.08%	0.009%
87	13.148	3747	3750	3751	rBV3	1495	815	0.03%	0.004%
88	13.222	3770	3773	3775	rBV4	1594	1085	0.04%	0.005%
89	13.402	3827	3829	3833	rVB5	2521	1725	0.07%	0.008%
90	13.424	3833	3836	3841	rBV7	1872	2091	0.09%	0.010%
91	13.534	3863	3870	3877	rBV	12116	16835	0.69%	0.083%
92	13.675	3911	3914	3918	rBV5	1804	1431	0.06%	0.007%
93	14.193	4072	4075	4078	rBV4	1599	1509	0.06%	0.007%
94	14.231	4085	4087	4090	rVB4	1792	978	0.04%	0.005%
95	14.247	4090	4092	4097	rBV5	1970	1561	0.06%	0.008%
96	14.321	4110	4115	4120	rBV9	2681	3057	0.13%	0.015%
97	14.350	4121	4124	4126	rBV4	1681	1275	0.05%	0.006%
98	14.379	4130	4133	4135	rBV3	1692	1342	0.06%	0.007%
99	14.530	4178	4180	4185	rBV4	1277	874	0.04%	0.004%
100	15.424	4454	4458	4462	rBV6	3087	3527	0.15%	0.017%


Sum of corrected areas: 20384483

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015292.D
Acq On : 30 Mar 2020 23:21
Operator : SY/MD
Sample : L1976-06 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

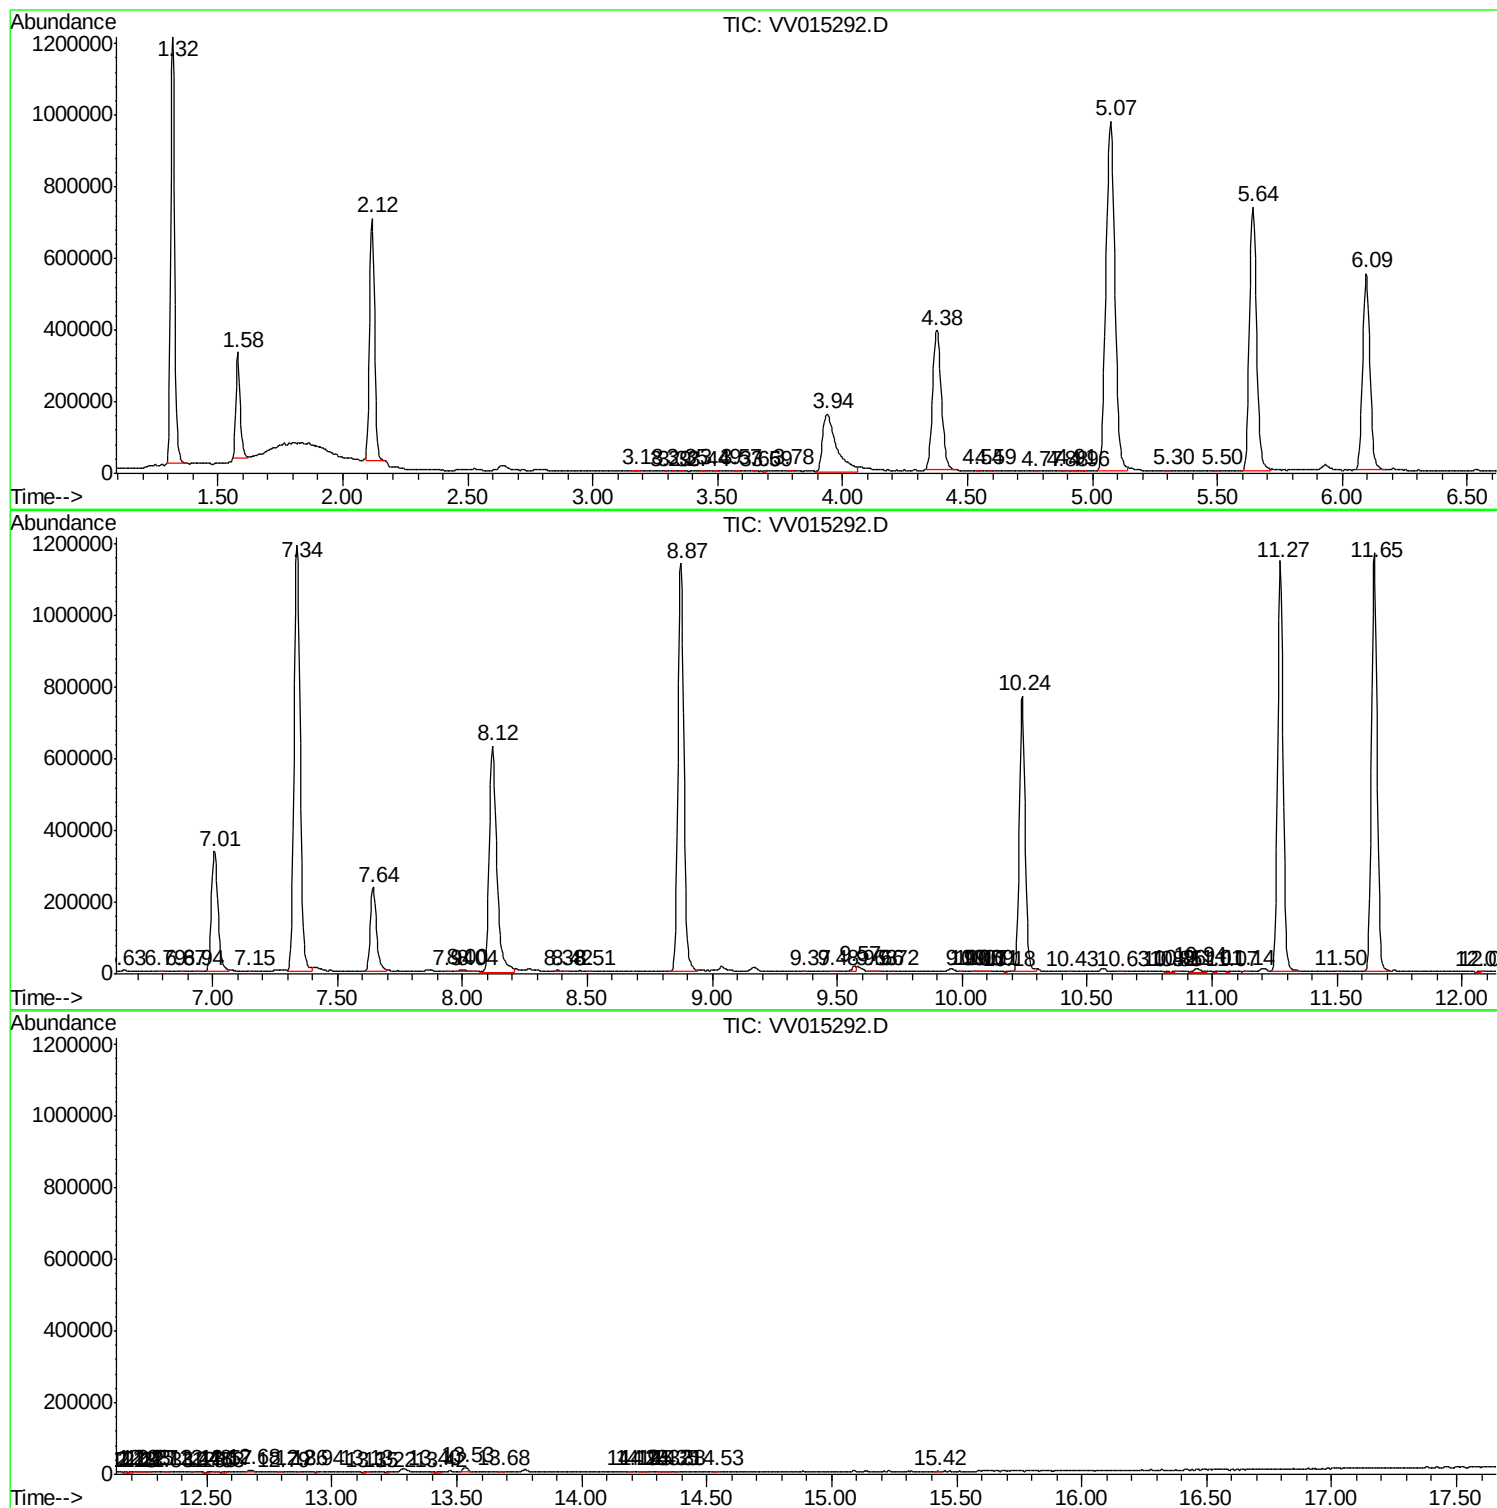

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015292.D
Acq On : 30 Mar 2020 23:21
Operator : SY/MD
Sample : L1976-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTLO

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033020\
Data File : VV015292.D
Acq On : 30 Mar 2020 23:21
Operator : SY/MD
Sample : L1976-06 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTLO

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc