

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015295.D
 Acq On : 31 Mar 2020 01:23
 Operator : SY/MD
 Sample : L1975-05 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	88	rVB2	881176	964236	22.73%	4.275%
2	1.579	146	152	165	rBV	293564	340626	8.03%	1.510%
3	2.119	313	320	353	rVB	652954	1010825	23.83%	4.482%
4	2.778	518	525	539	rVB7	10055	19271	0.45%	0.085%
5	3.065	612	614	617	rBV4	2159	1496	0.04%	0.007%
6	3.155	640	642	646	rBV5	2597	1873	0.04%	0.008%
7	3.322	692	694	699	rBV6	1304	835	0.02%	0.004%
8	3.823	848	850	852	rBV3	1666	906	0.02%	0.004%
9	3.939	869	886	928	rBV2	1669102	4241521	100.00%	18.807%
10	4.376	1009	1022	1048	rVB	363667	883314	20.83%	3.917%
11	4.592	1086	1089	1091	rBV3	1915	1352	0.03%	0.006%
12	4.769	1140	1144	1146	rBV5	1641	1182	0.03%	0.005%
13	5.000	1212	1216	1218	rBV5	1373	988	0.02%	0.004%
14	5.074	1219	1239	1272	rBV2	879539	2223767	52.43%	9.860%
15	5.302	1307	1310	1312	rBV3	1833	1187	0.03%	0.005%
16	5.357	1323	1327	1330	rBV5	1616	1248	0.03%	0.006%
17	5.489	1363	1368	1370	rBV5	2461	2070	0.05%	0.009%
18	5.511	1373	1375	1377	rBV3	1786	957	0.02%	0.004%
19	5.560	1387	1390	1392	rBV4	1904	1190	0.03%	0.005%
20	5.640	1401	1415	1435	rBV	735414	1470412	34.67%	6.520%
21	6.093	1540	1556	1581	rBV	490190	1016342	23.96%	4.506%
22	6.396	1646	1650	1652	rBV4	1978	1106	0.03%	0.005%
23	6.556	1697	1700	1704	rBV5	2918	1867	0.04%	0.008%
24	6.582	1704	1708	1709	rBV3	1324	996	0.02%	0.004%
25	6.627	1715	1722	1726	rBV7	2582	3828	0.09%	0.017%
26	6.743	1754	1758	1761	rBV6	2554	2502	0.06%	0.011%
27	6.778	1767	1769	1774	rVB5	1565	943	0.02%	0.004%
28	6.891	1800	1804	1807	rVB5	2192	1802	0.04%	0.008%
29	6.907	1807	1809	1812	rBV3	2051	1223	0.03%	0.005%
30	7.007	1829	1840	1864	rBV	300006	541152	12.76%	2.399%
31	7.338	1930	1943	1963	rBV	1100406	1886538	44.48%	8.365%
32	7.643	2028	2038	2053	rBV	204308	349110	8.23%	1.548%
33	8.116	2174	2185	2214	rBV	581184	1142188	26.93%	5.064%
34	8.514	2307	2309	2316	rBV9	1978	2333	0.06%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015295.D
 Acq On : 31 Mar 2020 01:23
 Operator : SY/MD
 Sample : L1975-05 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	8.621	2339	2342	2346	rBV6	2064	1827	0.04%	0.008%
36	8.640	2346	2348	2352	rVB4	1968	1290	0.03%	0.006%
37	8.775	2387	2390	2391	rBV4	1395	773	0.02%	0.003%
38	8.875	2408	2421	2440	rBV	1170857	1881183	44.35%	8.341%
39	9.222	2527	2529	2532	rVB3	2289	1228	0.03%	0.005%
40	9.264	2535	2542	2546	rBV7	2914	4013	0.09%	0.018%
41	9.289	2546	2550	2552	rBV4	2060	1518	0.04%	0.007%
42	9.505	2615	2617	2621	rBV4	1225	1116	0.03%	0.005%
43	9.649	2659	2662	2665	rBV4	1377	1124	0.03%	0.005%
44	9.733	2685	2688	2690	rBV3	1629	1019	0.02%	0.005%
45	9.810	2708	2712	2714	rBV5	2688	1891	0.04%	0.008%
46	9.836	2718	2720	2721	rVV2	2060	925	0.02%	0.004%
47	9.878	2731	2733	2737	rBV4	2050	1169	0.03%	0.005%
48	9.897	2737	2739	2745	rBV6	2363	2312	0.05%	0.010%
49	10.029	2776	2780	2782	rBV5	2054	1357	0.03%	0.006%
50	10.119	2805	2808	2809	rBV3	2093	1027	0.02%	0.005%
51	10.238	2834	2845	2862	rBV	683015	1065712	25.13%	4.725%
52	10.373	2884	2887	2894	rBV8	2014	2348	0.06%	0.010%
53	10.547	2937	2941	2943	rBV4	1257	1005	0.02%	0.004%
54	10.604	2957	2959	2963	rBV4	1360	1195	0.03%	0.005%
55	10.682	2978	2983	2988	rVB7	2459	2560	0.06%	0.011%
56	10.707	2988	2991	2994	rBV5	1243	1081	0.03%	0.005%
57	10.759	3004	3007	3011	rBV5	1576	1332	0.03%	0.006%
58	10.794	3016	3018	3022	rBV5	1269	799	0.02%	0.004%
59	10.855	3034	3037	3039	rBV4	1138	770	0.02%	0.003%
60	10.868	3039	3041	3044	rBV4	1437	869	0.02%	0.004%
61	10.920	3053	3057	3059	rBV5	2459	1704	0.04%	0.008%
62	11.013	3080	3086	3089	rBV8	1508	1699	0.04%	0.008%
63	11.077	3102	3106	3109	rVV5	2031	1495	0.04%	0.007%
64	11.186	3137	3140	3143	rBV4	2214	1661	0.04%	0.007%
65	11.273	3155	3167	3194	rBV	1134253	1748524	41.22%	7.753%
66	11.408	3207	3209	3213	rBV4	1567	837	0.02%	0.004%
67	11.495	3233	3236	3238	rBV4	1556	850	0.02%	0.004%
68	11.601	3267	3269	3272	rBV4	2041	1321	0.03%	0.006%
69	11.649	3272	3284	3300	rVV	1074656	1649299	38.88%	7.313%
70	11.858	3346	3349	3350	rBV3	1961	1053	0.02%	0.005%
71	11.919	3363	3368	3369	rBV6	1498	1283	0.03%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015295.D
 Acq On : 31 Mar 2020 01:23
 Operator : SY/MD
 Sample : L1975-05 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.997	3389	3392	3394	rVB4	1867	1156	0.03%	0.005%
73	12.029	3399	3402	3405	rBV4	2140	1703	0.04%	0.008%
74	12.164	3441	3444	3447	rBV6	1637	1059	0.02%	0.005%
75	12.286	3478	3482	3490	rVB8	2084	1767	0.04%	0.008%
76	12.318	3490	3492	3496	rVB5	1752	1181	0.03%	0.005%
77	12.344	3496	3500	3502	rBV3	1792	1240	0.03%	0.005%
78	12.553	3561	3565	3569	rBV8	1351	895	0.02%	0.004%
79	12.601	3578	3580	3586	rBV6	1174	1069	0.03%	0.005%
80	12.640	3586	3592	3595	rBV7	2194	2201	0.05%	0.010%
81	12.794	3636	3640	3642	rBV5	2431	1628	0.04%	0.007%
82	12.890	3666	3670	3674	rBV7	2517	1747	0.04%	0.008%
83	13.038	3713	3716	3717	rBV2	1889	1192	0.03%	0.005%
84	13.074	3723	3727	3729	rBV4	1703	1329	0.03%	0.006%
85	13.122	3740	3742	3746	rVB5	2130	1192	0.03%	0.005%
86	13.145	3746	3749	3752	rBV5	912	827	0.02%	0.004%
87	13.354	3810	3814	3818	rBV6	2392	2193	0.05%	0.010%
88	13.373	3818	3820	3824	rVB5	1991	1585	0.04%	0.007%
89	13.444	3840	3842	3845	rVB4	1636	1021	0.02%	0.005%
90	13.752	3935	3938	3939	rBV3	1573	830	0.02%	0.004%
91	13.829	3959	3962	3966	rBV6	2206	1736	0.04%	0.008%
92	13.907	3985	3986	3989	rBV3	1474	862	0.02%	0.004%
93	14.051	4029	4031	4034	rBV4	1667	1243	0.03%	0.006%
94	14.148	4058	4061	4065	rBV6	1755	1689	0.04%	0.007%
95	14.254	4091	4094	4096	rBV4	1590	1147	0.03%	0.005%
96	14.321	4111	4115	4116	rBV3	1652	1279	0.03%	0.006%
97	14.479	4160	4164	4165	rBV4	1267	866	0.02%	0.004%
98	14.514	4171	4175	4179	rBV5	2482	2184	0.05%	0.010%
99	14.762	4247	4252	4253	rBV4	2226	1724	0.04%	0.008%
100	15.180	4379	4382	4384	rBV4	3515	2099	0.05%	0.009%


Sum of corrected areas: 22552999

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015295.D
Acq On : 31 Mar 2020 01:23
Operator : SY/MD
Sample : L1975-05 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

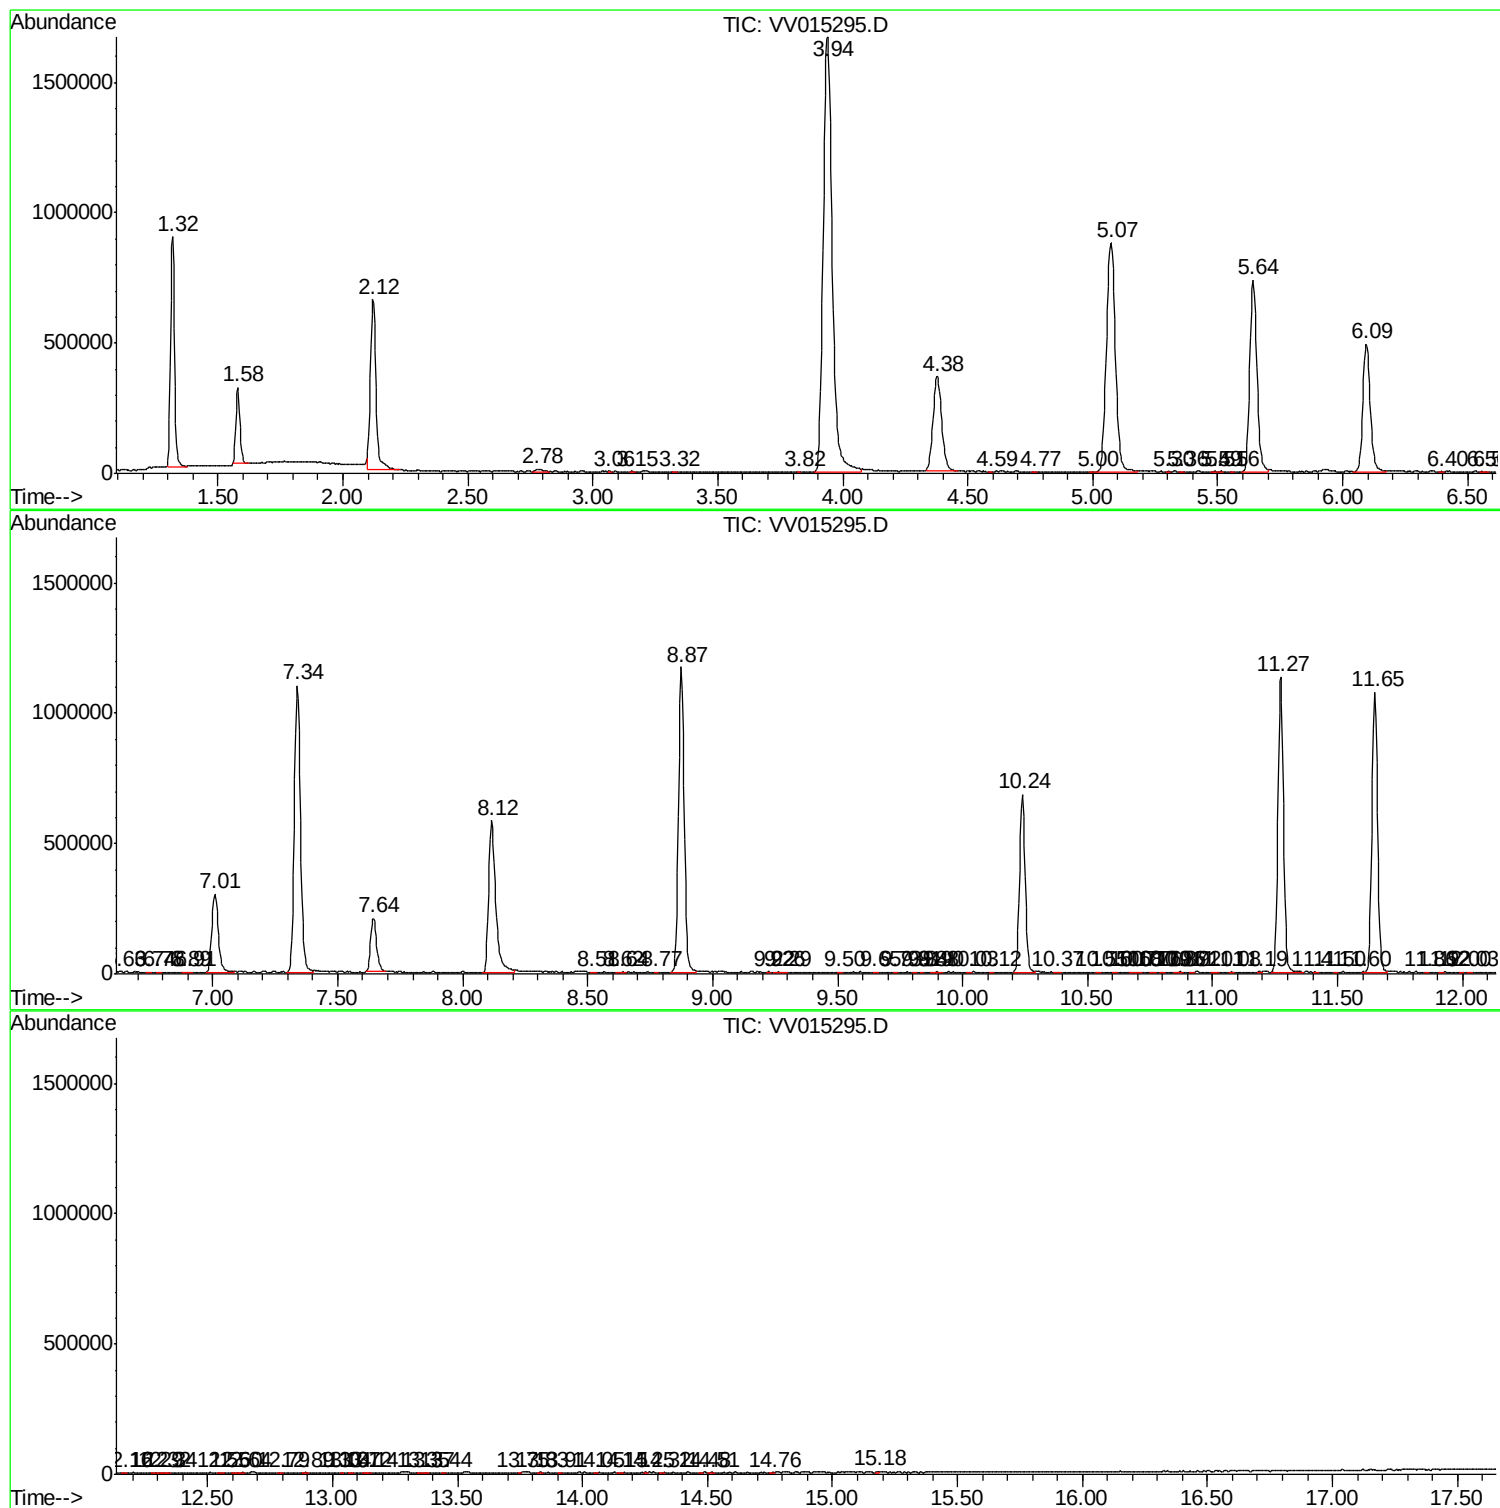

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015295.D
Acq On : 31 Mar 2020 01:23
Operator : SY/MD
Sample : L1975-05 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033020\
Data File : VV015295.D
Acq On : 31 Mar 2020 01:23
Operator : SY/MD
Sample : L1975-05 50X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTH0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc