

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015296.D
 Acq On : 31 Mar 2020 01:48
 Operator : SY/MD
 Sample : L1975-14 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	83	rVB2	806277	862405	28.63%	4.120%
2	1.579	146	152	162	rBV	285924	329017	10.92%	1.572%
3	2.119	313	320	339	rVB	639884	937985	31.14%	4.481%
4	2.862	549	551	553	rBV3	1555	637	0.02%	0.003%
5	3.016	597	599	603	rVB4	2033	1023	0.03%	0.005%
6	3.151	639	641	643	rBV3	1408	617	0.02%	0.003%
7	3.235	665	667	668	rBV2	1051	515	0.02%	0.002%
8	3.261	674	675	677	rBV2	1652	628	0.02%	0.003%
9	3.319	691	693	698	rBV5	1665	1169	0.04%	0.006%
10	3.508	748	752	753	rBV3	2176	1747	0.06%	0.008%
11	3.560	766	768	774	rVB6	2461	1833	0.06%	0.009%
12	3.582	774	775	777	rBV2	1498	758	0.03%	0.004%
13	3.659	797	799	805	rVB7	2391	1613	0.05%	0.008%
14	3.685	805	807	809	rVB3	1246	521	0.02%	0.002%
15	3.698	809	811	812	rBV2	1180	501	0.02%	0.002%
16	3.794	839	841	842	rBV2	597	201	0.01%	0.001%
17	3.804	842	844	849	rBV5	1541	1496	0.05%	0.007%
18	3.936	866	885	919	rBV2	1163620	3012320	100.00%	14.390%
19	4.376	1009	1022	1049	rVB	363410	893919	29.68%	4.270%
20	4.791	1149	1151	1152	rBV	1487	600	0.02%	0.003%
21	4.897	1181	1184	1186	rBV4	1600	1024	0.03%	0.005%
22	5.000	1213	1216	1220	rBV5	2408	1963	0.07%	0.009%
23	5.071	1221	1238	1270	rVV2	887804	2228369	73.98%	10.645%
24	5.640	1403	1415	1435	rBV	710369	1396249	46.35%	6.670%
25	6.093	1543	1556	1577	rBV	503849	1022272	33.94%	4.883%
26	6.489	1677	1679	1683	rBV5	2161	1307	0.04%	0.006%
27	6.566	1701	1703	1705	rBV2	1563	670	0.02%	0.003%
28	6.833	1781	1786	1788	rBV6	1127	990	0.03%	0.005%
29	6.910	1807	1810	1814	rVB5	1777	1091	0.04%	0.005%
30	6.949	1819	1822	1825	rBV4	1927	1321	0.04%	0.006%
31	7.007	1829	1840	1860	rBV	298121	542974	18.03%	2.594%
32	7.338	1931	1943	1967	rBV	1115337	1898295	63.02%	9.068%
33	7.643	2027	2038	2053	rBV	213228	362904	12.05%	1.734%
34	7.952	2132	2134	2135	rBV2	1635	654	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015296.D
 Acq On : 31 Mar 2020 01:48
 Operator : SY/MD
 Sample : L1975-14 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	8.023	2154	2156	2159	rVB4	1183	452	0.02%	0.002%
36	8.116	2174	2185	2214	rBV	606090	1213533	40.29%	5.797%
37	8.656	2351	2353	2357	rBV4	1478	1170	0.04%	0.006%
38	8.682	2360	2361	2363	rBV2	968	457	0.02%	0.002%
39	8.875	2409	2421	2442	rBV	1099084	1771566	58.81%	8.463%
40	9.370	2573	2575	2578	rBV4	1159	966	0.03%	0.005%
41	9.457	2599	2602	2605	rBV4	1390	953	0.03%	0.005%
42	9.482	2608	2610	2612	rBV3	1869	1231	0.04%	0.006%
43	9.531	2623	2625	2628	rBV4	1600	781	0.03%	0.004%
44	9.621	2651	2653	2655	rVB3	1560	664	0.02%	0.003%
45	9.633	2655	2657	2658	rBV2	1118	510	0.02%	0.002%
46	9.662	2664	2666	2667	rBV2	1188	510	0.02%	0.002%
47	9.756	2693	2695	2696	rBV2	1133	415	0.01%	0.002%
48	9.830	2715	2718	2720	rVB3	1356	691	0.02%	0.003%
49	9.897	2736	2739	2745	rVB8	1975	1668	0.06%	0.008%
50	10.045	2779	2785	2788	rBV6	1624	1361	0.05%	0.007%
51	10.064	2788	2791	2792	rBV2	961	519	0.02%	0.002%
52	10.119	2805	2808	2814	rBV7	2866	2581	0.09%	0.012%
53	10.238	2834	2845	2861	rBV	702551	1091524	36.24%	5.214%
54	10.412	2896	2899	2900	rBV3	1551	904	0.03%	0.004%
55	10.453	2908	2912	2913	rBV3	928	580	0.02%	0.003%
56	10.498	2923	2926	2931	rBV7	2060	1761	0.06%	0.008%
57	10.614	2960	2962	2963	rBV	1476	811	0.03%	0.004%
58	10.685	2983	2984	2989	rVB4	1887	1249	0.04%	0.006%
59	10.707	2989	2991	2992	rBV2	1034	377	0.01%	0.002%
60	10.765	3006	3009	3010	rBV3	1231	657	0.02%	0.003%
61	10.788	3014	3016	3019	rVV5	2048	1284	0.04%	0.006%
62	10.817	3023	3025	3028	rVB2	1511	733	0.02%	0.004%
63	10.833	3028	3030	3034	rBV4	859	490	0.02%	0.002%
64	10.900	3048	3051	3053	rBV3	1223	801	0.03%	0.004%
65	11.006	3082	3084	3086	rBV3	1450	630	0.02%	0.003%
66	11.045	3095	3096	3100	rVB3	1891	654	0.02%	0.003%
67	11.074	3100	3105	3107	rBV5	2243	2088	0.07%	0.010%
68	11.158	3126	3131	3132	rBV4	1622	1311	0.04%	0.006%
69	11.273	3155	3167	3184	rBV	1078393	1643317	54.55%	7.850%
70	11.463	3224	3226	3227	rBV2	709	284	0.01%	0.001%
71	11.576	3254	3261	3267	rBV2	3208	4611	0.15%	0.022%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015296.D
 Acq On : 31 Mar 2020 01:48
 Operator : SY/MD
 Sample : L1975-14 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.646	3272	3283	3298	rVV	1041412	1637138	54.35%	7.821%
73	11.820	3334	3337	3341	rBV4	1465	1260	0.04%	0.006%
74	11.916	3364	3367	3368	rBV3	1840	996	0.03%	0.005%
75	12.013	3396	3397	3399	rBV2	809	362	0.01%	0.002%
76	12.045	3404	3407	3409	rBV3	1527	930	0.03%	0.004%
77	12.096	3421	3423	3424	rBV	1422	427	0.01%	0.002%
78	12.119	3429	3430	3432	rBV2	1290	489	0.02%	0.002%
79	12.157	3439	3442	3445	rBV4	2232	1497	0.05%	0.007%
80	12.244	3465	3469	3471	rBV4	1196	1130	0.04%	0.005%
81	12.273	3475	3478	3480	rBV3	1246	793	0.03%	0.004%
82	12.624	3583	3587	3589	rBV6	1424	1074	0.04%	0.005%
83	12.900	3670	3673	3676	rVB5	1964	1180	0.04%	0.006%
84	12.993	3701	3702	3705	rVB3	1868	872	0.03%	0.004%
85	13.090	3728	3732	3735	rBV6	1963	1810	0.06%	0.009%
86	13.125	3741	3743	3750	rVB8	1093	1099	0.04%	0.005%
87	13.328	3802	3806	3811	rBV7	2086	2088	0.07%	0.010%
88	13.366	3812	3818	3821	rBV7	2694	2407	0.08%	0.011%
89	13.383	3821	3823	3824	rBV	947	355	0.01%	0.002%
90	13.482	3852	3854	3856	rVB3	1310	553	0.02%	0.003%
91	13.524	3864	3867	3868	rBV3	2922	1475	0.05%	0.007%
92	13.604	3890	3892	3893	rBV3	1908	818	0.03%	0.004%
93	13.717	3924	3927	3929	rBV4	1773	1219	0.04%	0.006%
94	14.026	4019	4023	4026	rBV4	2876	3167	0.11%	0.015%
95	14.103	4042	4047	4050	rBV7	2380	2688	0.09%	0.013%
96	14.193	4072	4075	4077	rBV3	2056	1136	0.04%	0.005%
97	14.241	4087	4090	4093	rBV4	2213	1798	0.06%	0.009%
98	14.791	4259	4261	4264	rBV4	1706	1454	0.05%	0.007%


Sum of corrected areas: 20933897

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015296.D
Acq On : 31 Mar 2020 01:48
Operator : SY/MD
Sample : L1975-14 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

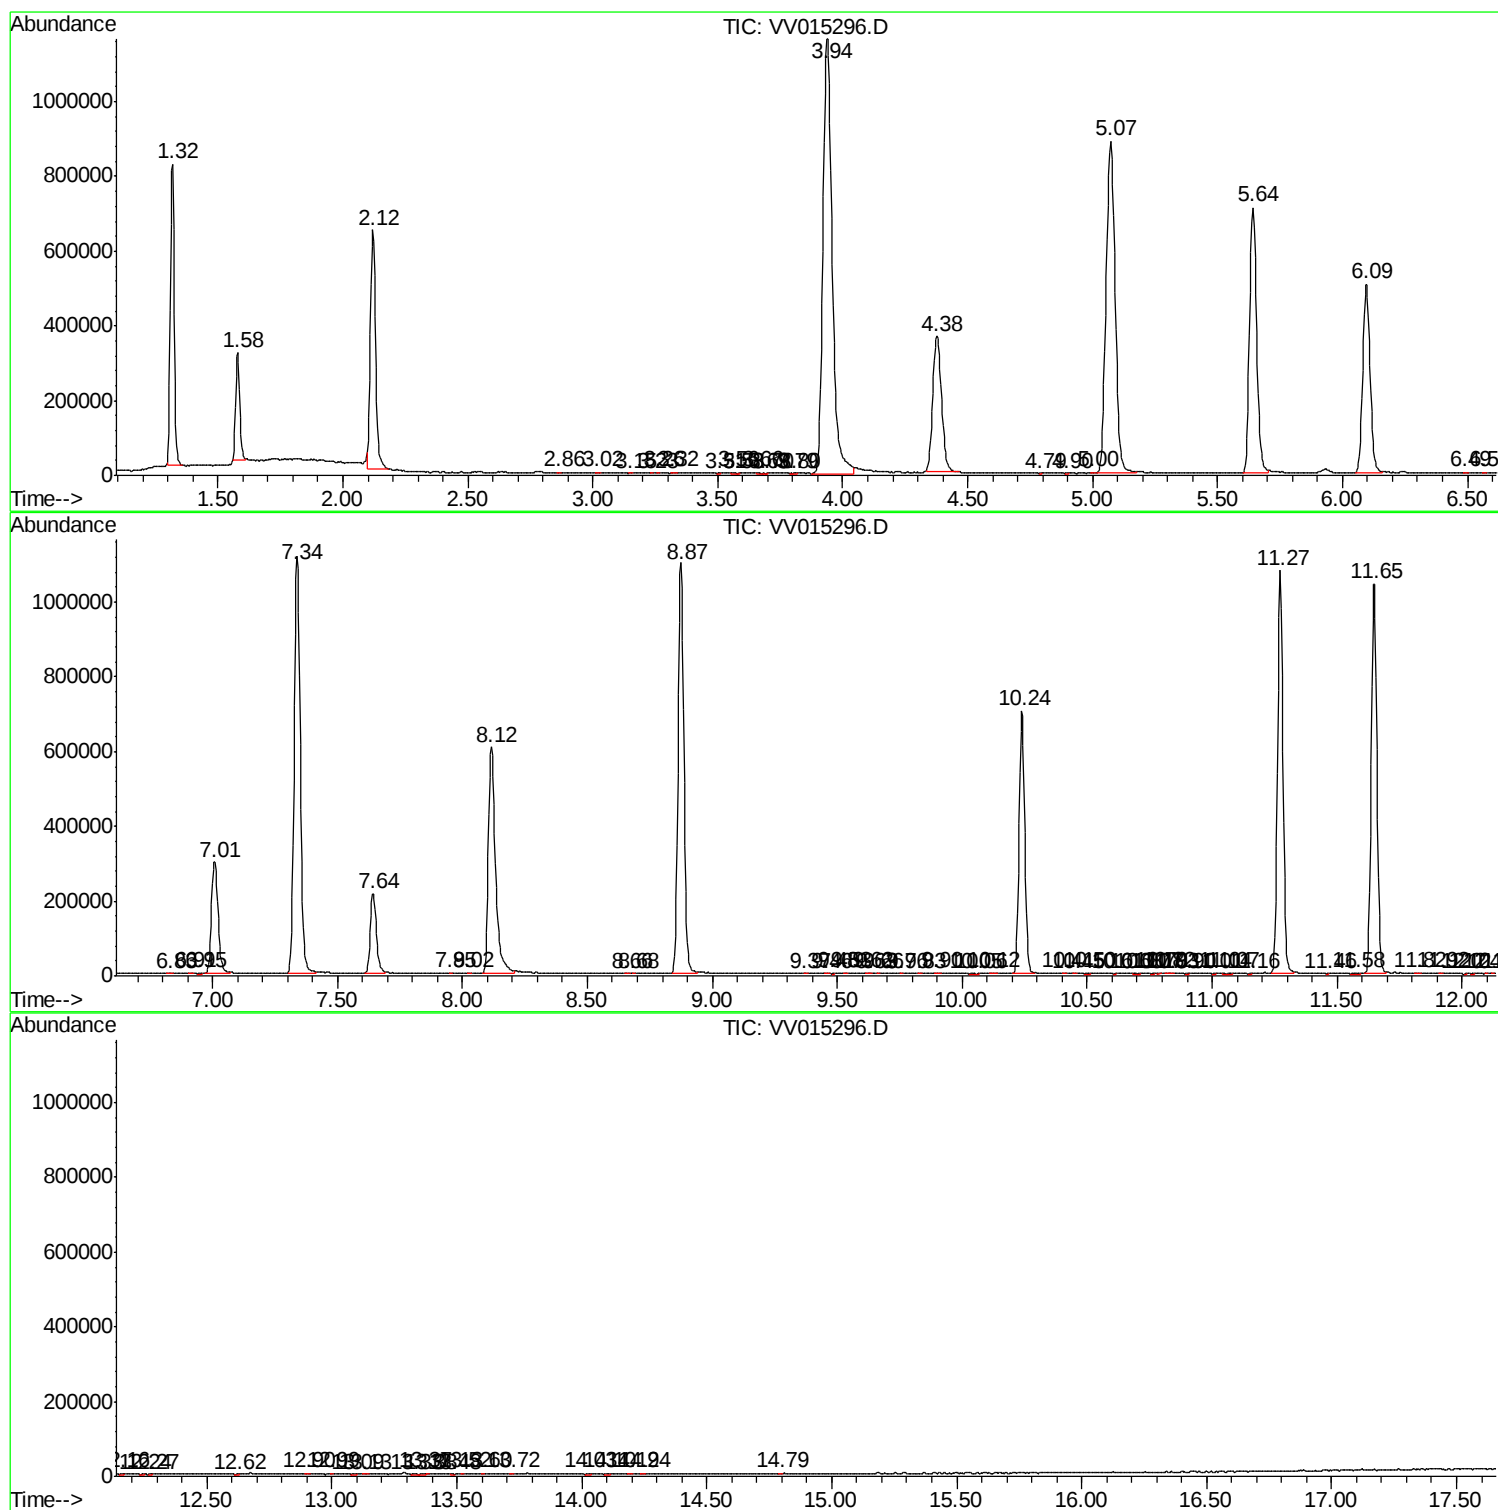

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015296.D
Acq On : 31 Mar 2020 01:48
Operator : SY/MD
Sample : L1975-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015296.D
Acq On : 31 Mar 2020 01:48
Operator : SY/MD
Sample : L1975-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc