

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015297.D
 Acq On : 31 Mar 2020 02:12
 Operator : SY/MD
 Sample : L1975-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	84	rVB2	576549	637174	27.17%	3.149%
2	1.579	146	152	166	rBV	296940	348598	14.86%	1.723%
3	2.122	313	321	346	rVB	625313	963822	41.09%	4.763%
4	3.074	611	617	622	rBV	2585	2539	0.11%	0.013%
5	3.180	646	650	652	rBV4	1888	1294	0.06%	0.006%
6	3.351	699	703	708	rBV8	2342	2784	0.12%	0.014%
7	3.399	716	718	719	rBV2	1413	613	0.03%	0.003%
8	3.428	723	727	729	rBV5	1186	971	0.04%	0.005%
9	3.444	729	732	734	rVV4	1784	955	0.04%	0.005%
10	3.515	751	754	759	rBV6	2162	1735	0.07%	0.009%
11	3.537	759	761	767	rVB6	2643	2174	0.09%	0.011%
12	3.737	820	823	824	rBV3	1989	910	0.04%	0.004%
13	3.862	858	862	863	rBV4	2647	1348	0.06%	0.007%
14	3.939	871	886	921	rBV2	883056	2345397	100.00%	11.591%
15	4.376	1006	1022	1042	rBV	363759	895547	38.18%	4.426%
16	4.669	1111	1113	1120	rBV7	2205	1821	0.08%	0.009%
17	4.782	1145	1148	1149	rBV3	1011	571	0.02%	0.003%
18	4.810	1153	1157	1159	rBV4	1693	1181	0.05%	0.006%
19	4.907	1185	1187	1188	rBV2	1487	632	0.03%	0.003%
20	5.074	1220	1239	1264	rBV2	882022	2227613	94.98%	11.009%
21	5.463	1356	1360	1364	rBV7	1691	1536	0.07%	0.008%
22	5.572	1392	1394	1396	rBV3	1880	774	0.03%	0.004%
23	5.643	1402	1416	1444	rBV	722657	1426575	60.82%	7.050%
24	5.810	1466	1468	1471	rVB3	2013	1202	0.05%	0.006%
25	5.933	1494	1506	1514	rBV3	12145	25320	1.08%	0.125%
26	6.007	1526	1529	1533	rBV5	2362	1303	0.06%	0.006%
27	6.097	1543	1557	1574	rBV	509612	1026613	43.77%	5.074%
28	6.338	1628	1632	1633	rBV3	1844	1282	0.05%	0.006%
29	6.598	1711	1713	1717	rBV5	1080	745	0.03%	0.004%
30	6.752	1756	1761	1768	rBV9	1871	3010	0.13%	0.015%
31	6.843	1787	1789	1790	rBV2	1458	600	0.03%	0.003%
32	6.884	1800	1802	1805	rVB3	1541	818	0.03%	0.004%
33	7.010	1830	1841	1859	rBV	301183	535180	22.82%	2.645%
34	7.338	1931	1943	1961	rBV	1095040	1881471	80.22%	9.298%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015297.D
 Acq On : 31 Mar 2020 02:12
 Operator : SY/MD
 Sample : L1975-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	7.643	2027	2038	2061	rBV	213798	368708	15.72%	1.822%
36	7.868	2107	2108	2110	rBV2	1032	481	0.02%	0.002%
37	8.116	2175	2185	2212	rBV	603852	1182206	50.41%	5.843%
38	8.524	2310	2312	2315	rBV4	1316	883	0.04%	0.004%
39	8.579	2326	2329	2331	rBV3	1880	1051	0.04%	0.005%
40	8.711	2368	2370	2373	rBV4	1370	776	0.03%	0.004%
41	8.730	2373	2376	2379	rVV5	1833	1309	0.06%	0.006%
42	8.759	2383	2385	2389	rVB4	1709	884	0.04%	0.004%
43	8.875	2407	2421	2442	rBV	1135140	1824559	77.79%	9.017%
44	9.186	2516	2518	2526	rVB9	3091	2431	0.10%	0.012%
45	9.309	2552	2556	2558	rBV5	2193	2076	0.09%	0.010%
46	9.350	2566	2569	2574	rBV7	1910	1566	0.07%	0.008%
47	9.531	2623	2625	2629	rBV5	1252	845	0.04%	0.004%
48	9.550	2629	2631	2633	rBV3	1683	835	0.04%	0.004%
49	9.604	2645	2648	2649	rBV2	1831	956	0.04%	0.005%
50	9.704	2677	2679	2685	rBV6	1966	2102	0.09%	0.010%
51	9.791	2703	2706	2708	rBV4	2566	1431	0.06%	0.007%
52	9.813	2711	2713	2718	rVB7	1750	1107	0.05%	0.005%
53	9.939	2750	2752	2755	rBV4	1648	770	0.03%	0.004%
54	9.987	2762	2767	2770	rBV6	2598	2440	0.10%	0.012%
55	10.003	2770	2772	2774	rBV4	1307	689	0.03%	0.003%
56	10.039	2779	2783	2784	rBV4	1574	1323	0.06%	0.007%
57	10.112	2804	2806	2811	rBV4	1623	1157	0.05%	0.006%
58	10.138	2811	2814	2818	rBV4	1997	1423	0.06%	0.007%
59	10.238	2833	2845	2862	rBV	706129	1107712	47.23%	5.474%
60	10.476	2914	2919	2920	rBV5	2185	1726	0.07%	0.009%
61	10.521	2929	2933	2935	rBV5	2062	1413	0.06%	0.007%
62	10.662	2975	2977	2978	rBV2	1695	683	0.03%	0.003%
63	10.833	3028	3030	3032	rBV3	1613	1012	0.04%	0.005%
64	10.878	3040	3044	3049	rBV8	1439	1553	0.07%	0.008%
65	10.929	3057	3060	3062	rBV3	2272	1480	0.06%	0.007%
66	10.997	3079	3081	3086	rVV5	2131	1773	0.08%	0.009%
67	11.045	3092	3096	3099	rBV5	1274	1012	0.04%	0.005%
68	11.061	3099	3101	3102	rBV	1583	494	0.02%	0.002%
69	11.174	3134	3136	3139	rBV3	1422	813	0.03%	0.004%
70	11.273	3155	3167	3185	rBV	1080664	1673340	71.35%	8.270%
71	11.518	3241	3243	3245	rBV3	1722	913	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015297.D
 Acq On : 31 Mar 2020 02:12
 Operator : SY/MD
 Sample : L1975-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.537	3247	3249	3252	rVB4	1228	700	0.03%	0.003%
73	11.649	3272	3284	3304	rBV	1070674	1659334	70.75%	8.201%
74	11.810	3331	3334	3336	rBV3	1725	1294	0.06%	0.006%
75	11.871	3351	3353	3354	rBV2	1233	527	0.02%	0.003%
76	11.897	3359	3361	3362	rBV2	1343	617	0.03%	0.003%
77	12.003	3387	3394	3397	rBV9	2208	2926	0.12%	0.014%
78	12.138	3434	3436	3439	rBV4	1368	1059	0.05%	0.005%
79	12.276	3477	3479	3481	rBV3	1814	860	0.04%	0.004%
80	12.360	3502	3505	3508	rBV4	1910	987	0.04%	0.005%
81	12.382	3510	3512	3516	rBV4	1227	1198	0.05%	0.006%
82	12.415	3520	3522	3524	rBV3	1622	621	0.03%	0.003%
83	12.447	3530	3532	3533	rBV2	1447	727	0.03%	0.004%
84	12.469	3537	3539	3545	rVV6	1885	1839	0.08%	0.009%
85	12.495	3545	3547	3554	rVB7	1243	1202	0.05%	0.006%
86	12.546	3561	3563	3567	rVB4	1144	780	0.03%	0.004%
87	12.739	3621	3623	3626	rBV4	1119	683	0.03%	0.003%
88	12.772	3631	3633	3639	rVB7	3396	2322	0.10%	0.011%
89	12.797	3639	3641	3644	rBV4	1317	711	0.03%	0.004%
90	13.077	3726	3728	3730	rBV3	1568	794	0.03%	0.004%
91	13.366	3814	3818	3819	rBV3	1160	844	0.04%	0.004%
92	13.424	3833	3836	3839	rBV5	2485	1484	0.06%	0.007%
93	13.460	3845	3847	3852	rVB5	2800	2008	0.09%	0.010%
94	13.739	3931	3934	3939	rBV7	3411	3494	0.15%	0.017%
95	13.964	4002	4004	4010	rVB6	1739	1162	0.05%	0.006%
96	14.022	4018	4022	4024	rBV4	1975	1623	0.07%	0.008%
97	14.161	4063	4065	4068	rBV4	1731	1091	0.05%	0.005%
98	14.222	4080	4084	4085	rBV3	2010	1646	0.07%	0.008%
99	14.283	4101	4103	4106	rBV3	1929	1000	0.04%	0.005%
100	14.646	4214	4216	4219	rBV3	1495	759	0.03%	0.004%


Sum of corrected areas: 20234332

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015297.D
Acq On : 31 Mar 2020 02:12
Operator : SY/MD
Sample : L1975-06 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

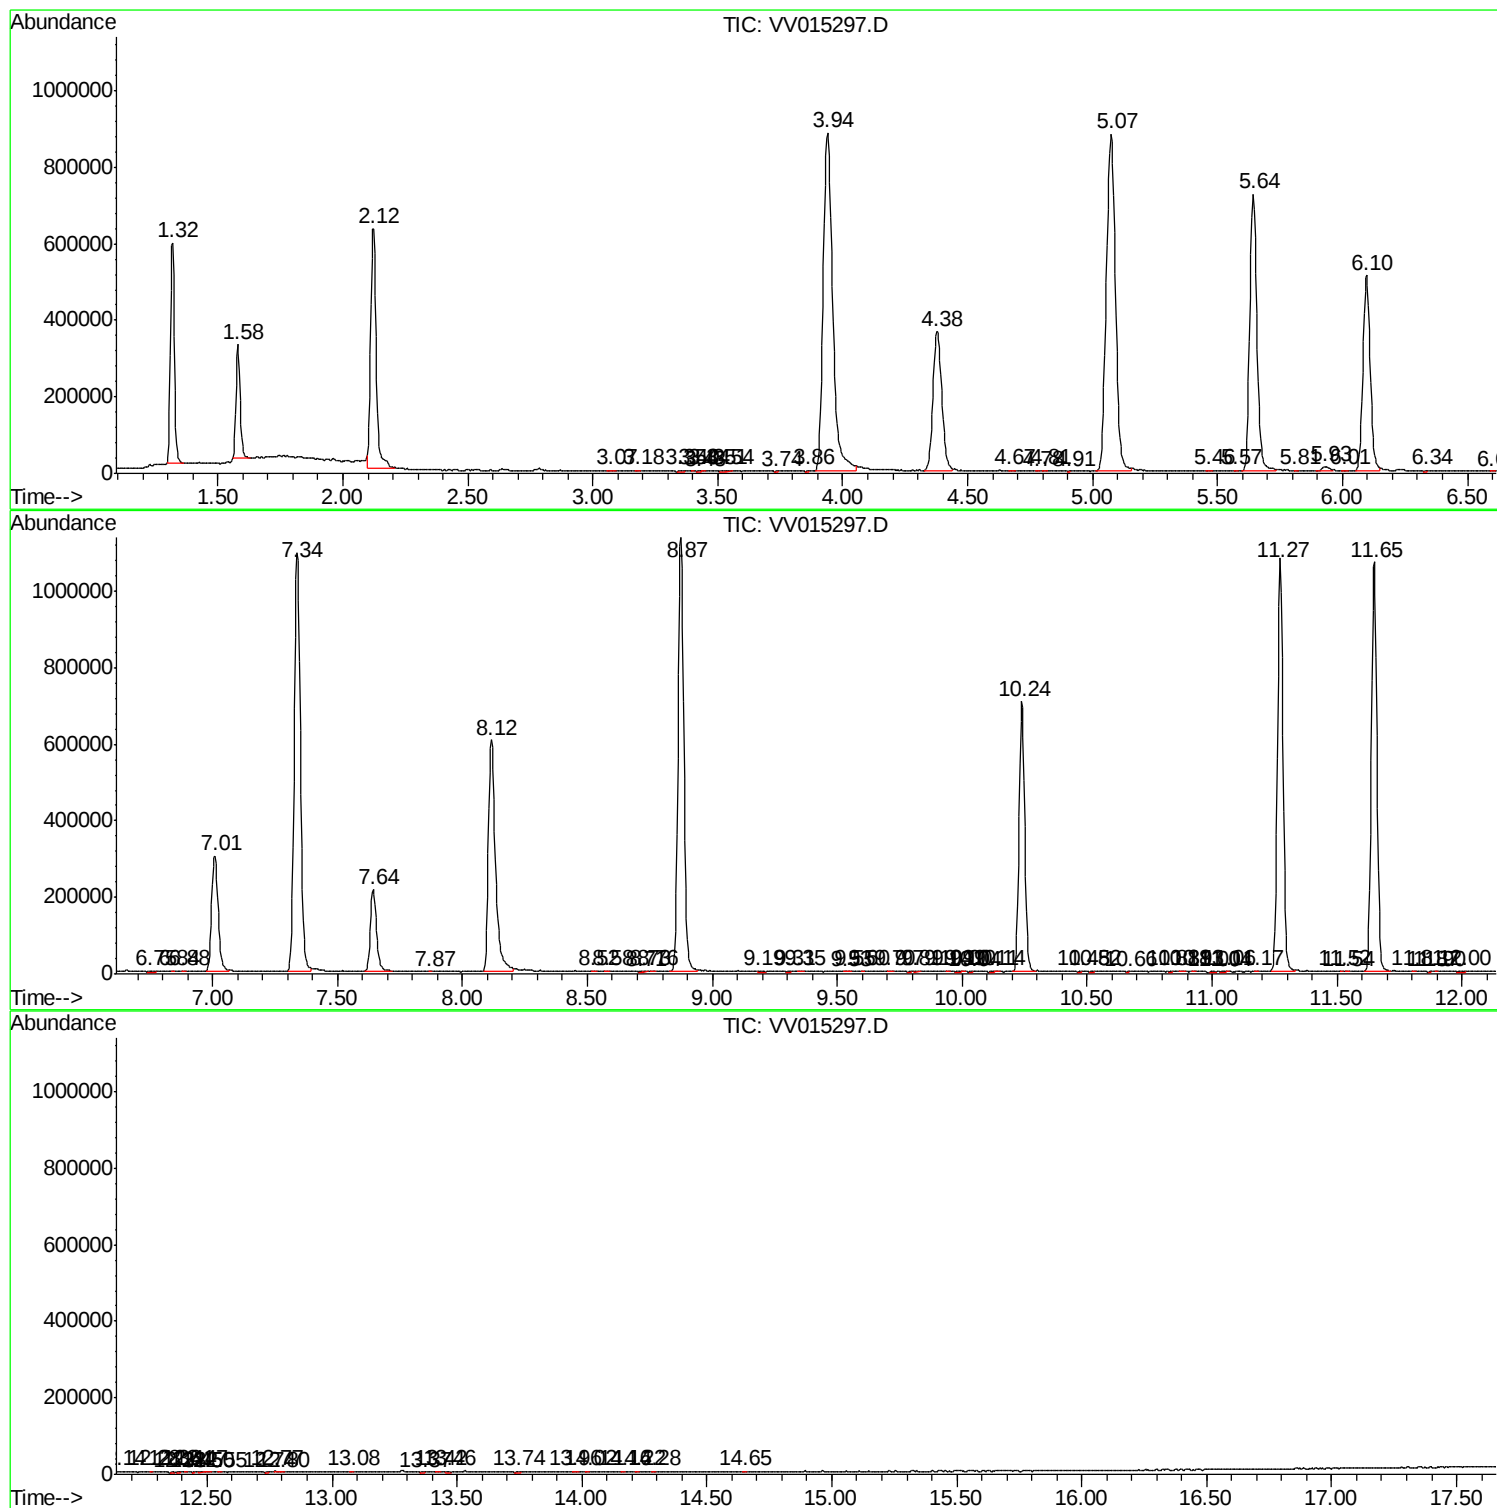

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015297.D
Acq On : 31 Mar 2020 02:12
Operator : SY/MD
Sample : L1975-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015297.D
Acq On : 31 Mar 2020 02:12
Operator : SY/MD
Sample : L1975-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc