

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015298.D
 Acq On : 31 Mar 2020 02:36
 Operator : SY/MD
 Sample : L1975-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB2	439322	464890	20.80%	2.539%
2	1.579	146	152	166	rVB	294380	344624	15.42%	1.882%
3	2.119	312	320	347	rVB	630846	967083	43.26%	5.283%
4	2.412	409	411	414	rBV3	2747	1929	0.09%	0.011%
5	2.518	439	444	445	rBV4	2771	2626	0.12%	0.014%
6	3.023	598	601	603	rVB4	1660	963	0.04%	0.005%
7	3.052	604	610	613	rBV6	2135	2222	0.10%	0.012%
8	3.171	644	647	649	rBV3	1929	1358	0.06%	0.007%
9	3.257	670	674	676	rBV4	2605	1133	0.05%	0.006%
10	3.466	737	739	742	rVV3	1693	768	0.03%	0.004%
11	3.511	751	753	756	rBV3	1560	881	0.04%	0.005%
12	3.560	766	768	772	rVB4	1456	981	0.04%	0.005%
13	3.679	803	805	808	rVB3	1740	761	0.03%	0.004%
14	3.701	808	812	814	rBV5	1346	1157	0.05%	0.006%
15	3.833	849	853	860	rBV7	2480	3039	0.14%	0.017%
16	3.865	860	863	866	rBV4	1777	1064	0.05%	0.006%
17	3.939	872	886	920	rBV3	237316	804492	35.99%	4.394%
18	4.376	1008	1022	1047	rVB	362159	884181	39.55%	4.830%
19	4.643	1102	1105	1108	rVB5	2066	1534	0.07%	0.008%
20	4.672	1112	1114	1115	rBV2	2265	987	0.04%	0.005%
21	4.714	1125	1127	1130	rBV4	1922	1015	0.05%	0.006%
22	4.753	1136	1139	1143	rBV5	2109	1541	0.07%	0.008%
23	5.071	1221	1238	1259	rBV2	889724	2235581	100.00%	12.212%
24	5.643	1403	1416	1439	rBV	684134	1365858	61.10%	7.461%
25	6.093	1543	1556	1575	rBV	507586	1021738	45.70%	5.581%
26	6.396	1647	1650	1654	rBV6	2048	1651	0.07%	0.009%
27	6.585	1706	1709	1711	rBV4	1258	820	0.04%	0.004%
28	6.756	1758	1762	1765	rBV4	1053	855	0.04%	0.005%
29	6.807	1775	1778	1782	rBV6	1684	1368	0.06%	0.007%
30	6.968	1825	1828	1829	rBV3	1663	996	0.04%	0.005%
31	7.010	1829	1841	1858	rVV	303022	539220	24.12%	2.945%
32	7.338	1931	1943	1963	rBV	1105834	1870076	83.65%	10.215%
33	7.553	2007	2010	2011	rBV3	2117	949	0.04%	0.005%
34	7.643	2028	2038	2064	rVB	214961	371269	16.61%	2.028%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015298.D
 Acq On : 31 Mar 2020 02:36
 Operator : SY/MD
 Sample : L1975-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	7.836	2095	2098	2100	rBV4	1725	1045	0.05%	0.006%
36	7.926	2124	2126	2128	rBV3	1913	1118	0.05%	0.006%
37	8.048	2162	2164	2169	rBV6	1149	899	0.04%	0.005%
38	8.116	2174	2185	2213	rBV	631170	1231749	55.10%	6.728%
39	8.331	2250	2252	2259	rBV7	2564	2856	0.13%	0.016%
40	8.582	2328	2330	2332	rBV2	1649	1003	0.04%	0.005%
41	8.720	2371	2373	2377	rBV4	2243	1823	0.08%	0.010%
42	8.801	2396	2398	2401	rVB3	1598	900	0.04%	0.005%
43	8.820	2401	2404	2405	rBV2	1236	781	0.03%	0.004%
44	8.875	2409	2421	2443	rBV	1086408	1728862	77.33%	9.444%
45	9.174	2508	2514	2519	rVV10	3279	4082	0.18%	0.022%
46	9.309	2552	2556	2559	rVB5	1574	1074	0.05%	0.006%
47	9.344	2563	2567	2568	rBV3	1259	776	0.03%	0.004%
48	9.363	2571	2573	2576	rBV4	1994	1016	0.05%	0.006%
49	9.405	2583	2586	2587	rBV2	1966	1004	0.04%	0.005%
50	9.437	2594	2596	2598	rBV3	1227	743	0.03%	0.004%
51	9.685	2668	2673	2674	rBV4	1453	1082	0.05%	0.006%
52	9.733	2685	2688	2689	rBV3	2268	1288	0.06%	0.007%
53	9.833	2714	2719	2720	rBV4	1992	1537	0.07%	0.008%
54	9.929	2746	2749	2750	rBV2	1492	809	0.04%	0.004%
55	9.987	2764	2767	2770	rBV6	1510	1139	0.05%	0.006%
56	10.151	2815	2818	2821	rVB4	2282	1489	0.07%	0.008%
57	10.238	2833	2845	2857	rBV	703222	1111684	49.73%	6.072%
58	10.334	2873	2875	2878	rBV4	1587	1019	0.05%	0.006%
59	10.714	2986	2993	2995	rBV7	2095	2166	0.10%	0.012%
60	10.942	3057	3064	3065	rBV6	2069	2166	0.10%	0.012%
61	11.074	3099	3105	3108	rBV7	2524	3066	0.14%	0.017%
62	11.273	3154	3167	3183	rBV	1043058	1593947	71.30%	8.707%
63	11.411	3206	3210	3213	rBV5	1823	1521	0.07%	0.008%
64	11.598	3265	3268	3271	rBV4	2826	2022	0.09%	0.011%
65	11.649	3271	3284	3300	rBV	1066658	1656374	74.09%	9.048%
66	11.887	3356	3358	3361	rBV4	2187	1462	0.07%	0.008%
67	11.910	3363	3365	3368	rBV3	1683	1241	0.06%	0.007%
68	11.955	3376	3379	3381	rBV4	1602	1077	0.05%	0.006%
69	12.045	3404	3407	3408	rBV3	2307	1355	0.06%	0.007%
70	12.096	3419	3423	3426	rVB4	1418	965	0.04%	0.005%
71	12.125	3430	3432	3437	rVV6	1528	1188	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033020\
 Data File : VV015298.D
 Acq On : 31 Mar 2020 02:36
 Operator : SY/MD
 Sample : L1975-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	12.173	3444	3447	3450	rBV5	1281	763	0.03%	0.004%
73	12.193	3451	3453	3455	rVV3	1649	723	0.03%	0.004%
74	12.337	3496	3498	3501	rBV4	1496	977	0.04%	0.005%
75	12.476	3538	3541	3544	rVB5	1722	907	0.04%	0.005%
76	12.505	3544	3550	3553	rBV8	2048	2301	0.10%	0.013%
77	12.575	3569	3572	3574	rBV3	1188	751	0.03%	0.004%
78	12.620	3583	3586	3591	rBV7	1356	1126	0.05%	0.006%
79	12.646	3591	3594	3596	rBV4	1365	777	0.03%	0.004%
80	12.945	3685	3687	3690	rVV4	2131	1014	0.05%	0.006%
81	13.103	3733	3736	3738	rBV4	2378	1795	0.08%	0.010%
82	13.202	3764	3767	3772	rVB7	2160	2093	0.09%	0.011%
83	13.231	3772	3776	3778	rBV5	1999	1413	0.06%	0.008%
84	13.289	3792	3794	3799	rVB5	2547	1908	0.09%	0.010%
85	13.456	3839	3846	3847	rBV6	2251	2060	0.09%	0.011%
86	13.540	3867	3872	3876	rVB8	2878	2177	0.10%	0.012%
87	13.604	3887	3892	3895	rBV7	1974	1754	0.08%	0.010%
88	13.627	3896	3899	3903	rVB5	1862	1641	0.07%	0.009%
89	13.672	3910	3913	3915	rVB4	2118	926	0.04%	0.005%
90	13.839	3963	3965	3969	rBV5	1627	768	0.03%	0.004%
91	13.984	4008	4010	4012	rVV3	2117	840	0.04%	0.005%
92	14.006	4013	4017	4022	rVB7	2303	2040	0.09%	0.011%
93	14.083	4039	4041	4044	rBV3	2370	965	0.04%	0.005%
94	14.225	4083	4085	4088	rBV4	1735	809	0.04%	0.004%
95	14.260	4094	4096	4100	rBV5	2131	1692	0.08%	0.009%
96	14.376	4130	4132	4137	rVB6	2217	1276	0.06%	0.007%
97	14.443	4150	4153	4160	rBV9	1826	1926	0.09%	0.011%
98	14.688	4227	4229	4236	rVB7	1600	1306	0.06%	0.007%
99	14.826	4270	4272	4275	rBV4	1690	1021	0.05%	0.006%
100	14.845	4275	4278	4282	rVV5	1460	1257	0.06%	0.007%


Sum of corrected areas: 18306944

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033020\
Data File : VV015298.D
Acq On : 31 Mar 2020 02:36
Operator : SY/MD
Sample : L1975-08 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

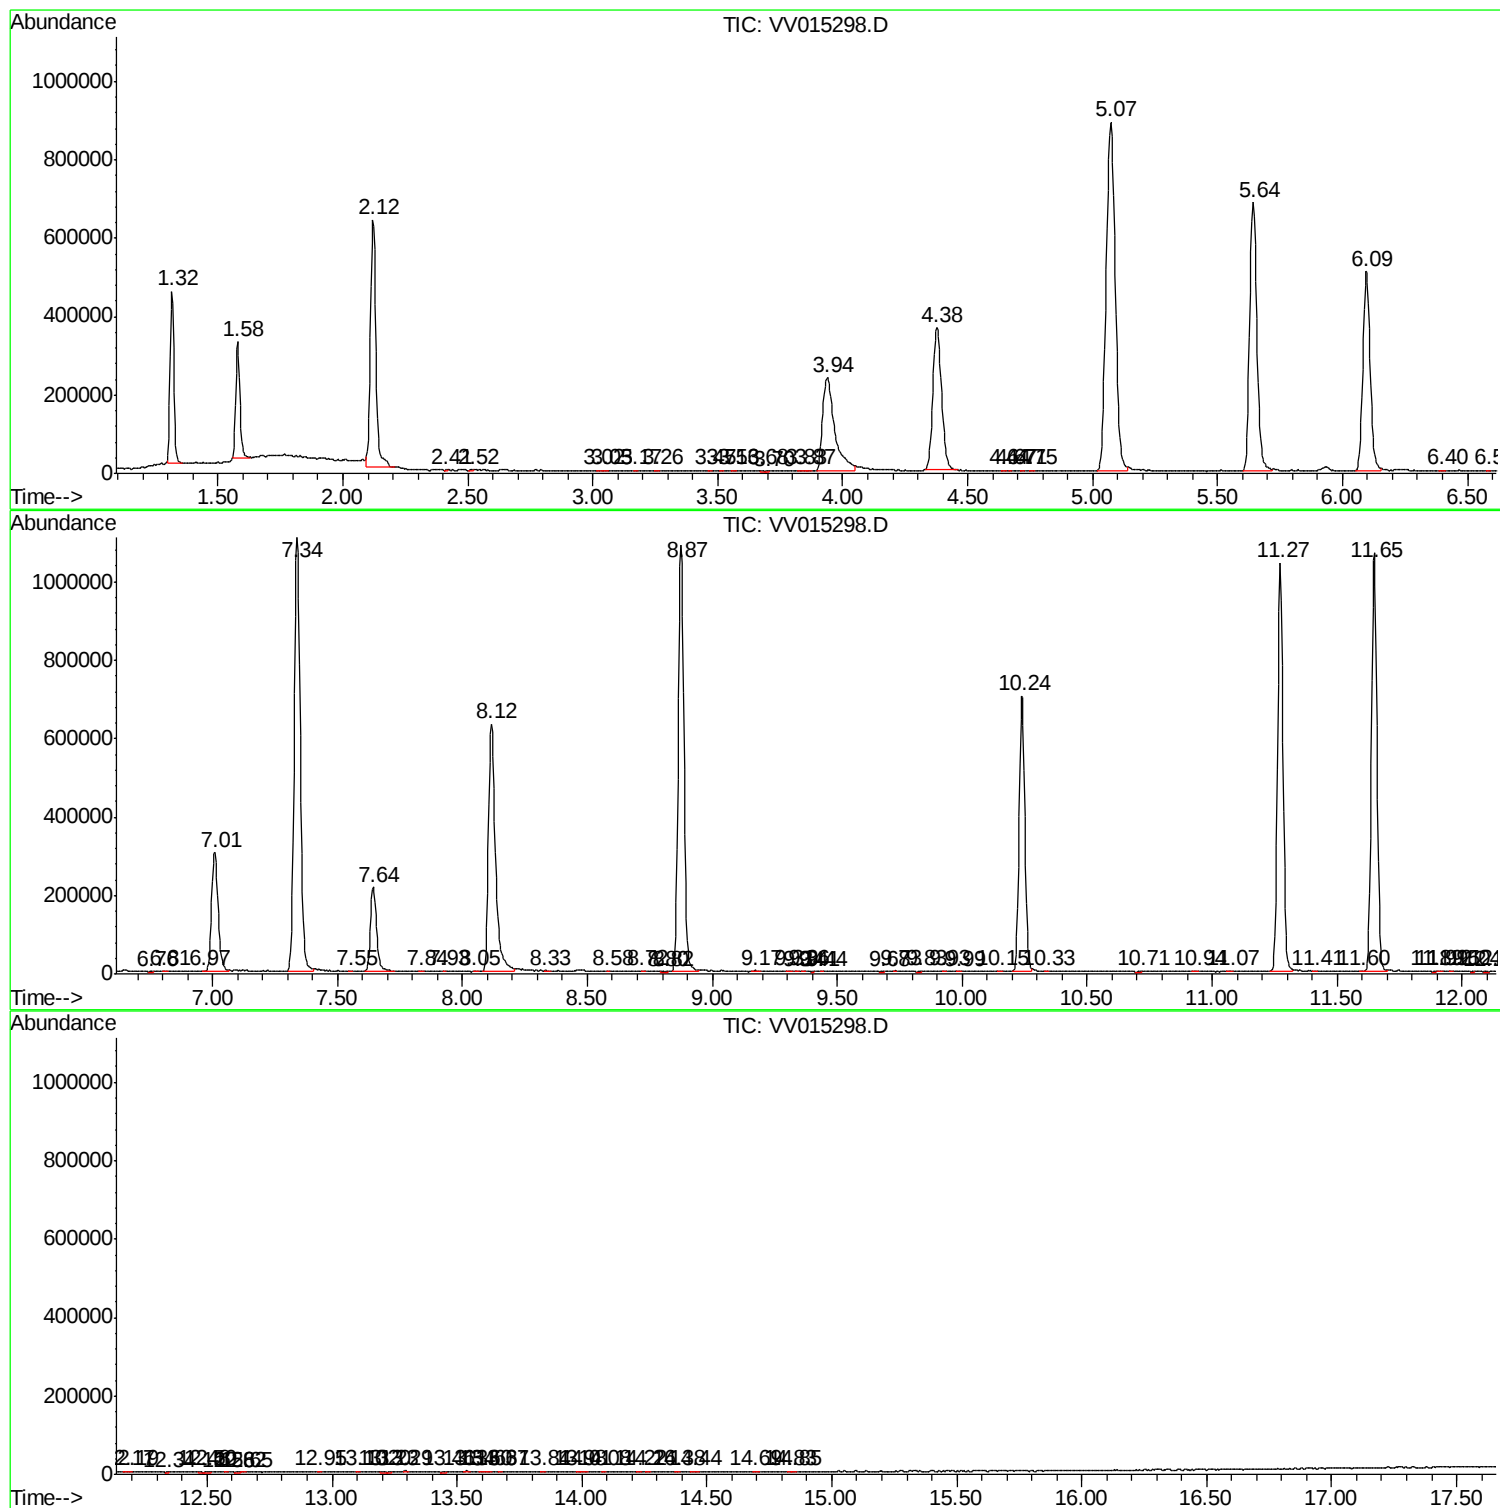

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033020\
Data File : VV015298.D
Acq On : 31 Mar 2020 02:36
Operator : SY/MD
Sample : L1975-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033020\
Data File : VV015298.D
Acq On : 31 Mar 2020 02:36
Operator : SY/MD
Sample : L1975-08 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc