


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV033020\
 Data File : VV015260.D
 Acq On : 30 Mar 2020 08:14
 Operator : SY/MD
 Sample : BFB74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB74

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 04 13:33:36 2020

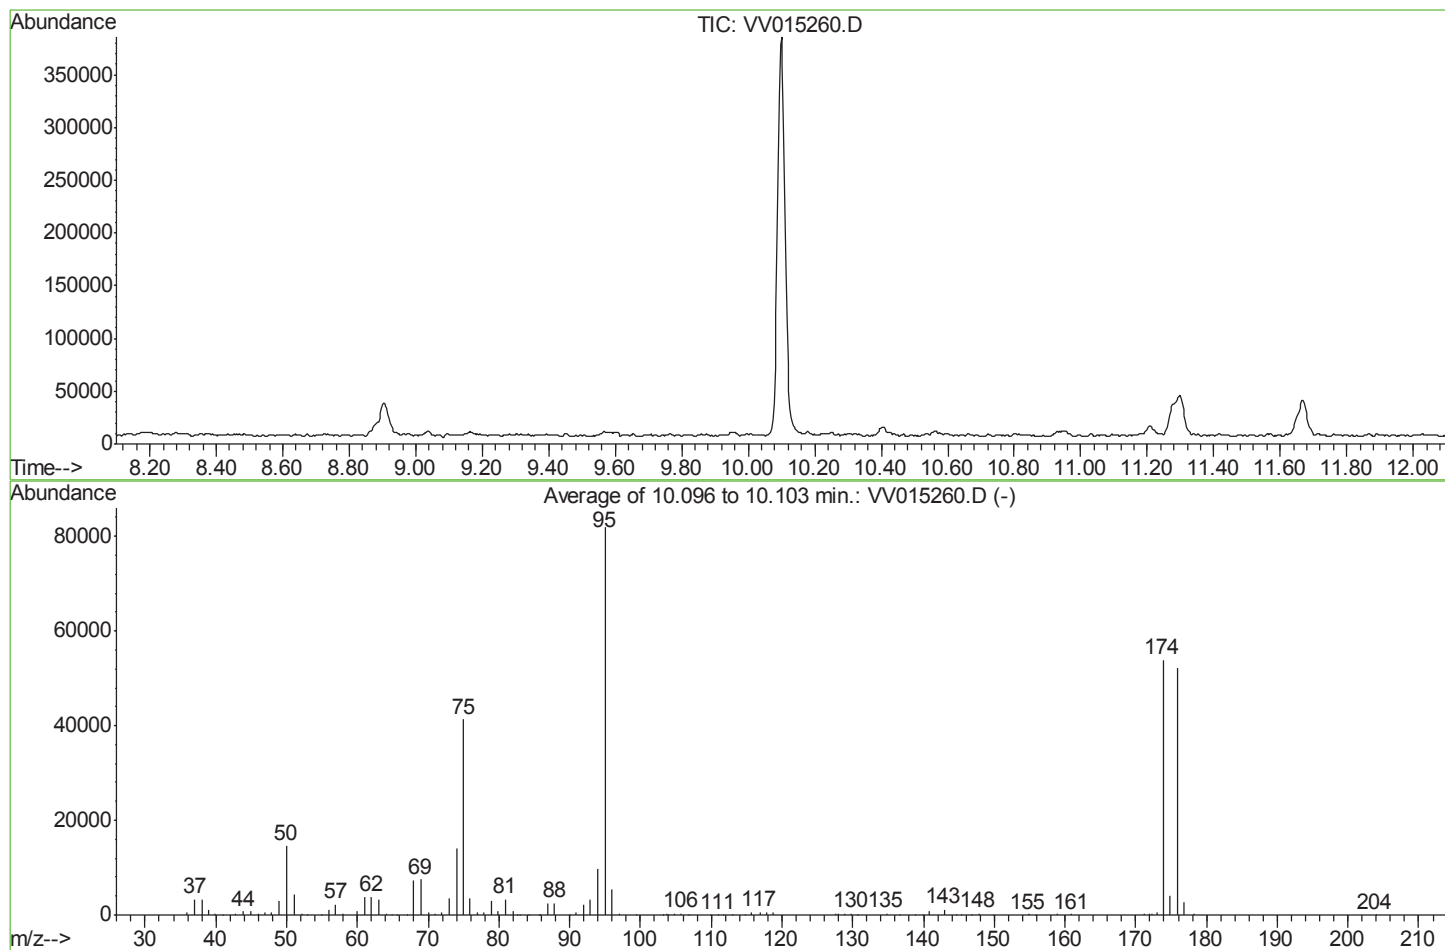

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2787

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	14623	PASS
75	95	30	80	50.5	41353	PASS
95	95	100	100	100.0	81898	PASS
96	95	5	9	6.7	5454	PASS
173	174	0.00	2	1.1	613	PASS
174	95	50	120	65.8	53920	PASS
175	174	5	9	7.5	4046	PASS
176	174	95	101	96.7	52162	PASS
177	176	5	9	5.5	2847	PASS

m/z	Abundance
35.90	537.0
37.00	3420.0
38.00	3521.0
39.00	1452.0
40.00	810.0
40.90	394.0
41.90	213.0
42.80	206.0
43.90	1353.0
44.90	749.0
46.00	266.0
47.00	612.0
47.90	437.0
48.90	3217.0
50.00	14615.0
51.00	3989.0
52.10	295.0
52.90	195.0
53.80	183.0
55.00	424.0
55.90	1333.0
56.90	2341.0
57.90	255.0
60.00	837.0
61.00	3797.0
62.00	3988.0
63.00	3423.0
64.00	400.0
64.80	140.0
65.60	125.0
67.10	243.0
68.00	7955.0
69.00	8576.0
70.00	806.0
71.00	212.0
72.00	501.0
73.00	3559.0
74.00	14366.0
75.00	42608.0
76.00	3763.0
77.00	629.0
77.90	319.0
78.90	3410.0
79.90	887.0
80.90	3571.0
82.00	921.0
82.90	192.0
84.30	189.0
85.70	113.0
86.90	2484.0
87.80	2640.0
91.00	336.0
91.90	2126.0
92.90	3222.0
94.00	9644.0
95.00	82632.0
96.00	5657.0
97.00	207.0
103.10	118.0
103.70	444.0
104.90	333.0
105.80	406.0
106.70	122.0
109.80	156.0
111.00	151.0
115.70	444.0
116.90	561.0
117.90	505.0
118.80	604.0
127.50	118.0
128.00	313.0
128.70	179.0
129.90	281.0
130.70	130.0
134.80	300.0
138.90	113.0
139.90	134.0
140.80	908.0
142.90	1131.0
144.70	124.0
145.40	113.0
147.80	189.0
149.80	134.0
154.90	226.0
155.70	101.0
159.00	178.0
161.00	167.0
171.20	128.0
171.80	257.0
173.00	608.0
173.90	53896.0
174.90	4094.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

175.90

176.90

178.30

52240.0

2812.0

191.0

Instrument :

MSVOA_V

ClientSampleId :

BFB74

m/z	Abundance
36.00	563.0
37.00	3498.0
38.00	3613.0
39.00	1518.0
39.90	787.0
40.90	451.0
41.90	211.0
42.70	241.0
43.90	1440.0
44.90	678.0
46.00	364.0
47.00	658.0
47.90	450.0
49.00	3106.0
50.00	15007.0
51.00	4335.0
52.10	238.0
52.90	242.0
53.80	209.0
55.00	493.0
55.90	1364.0
57.00	2432.0
57.90	268.0
59.90	853.0
60.90	3873.0
62.00	4026.0
63.00	3447.0
64.10	369.0
64.80	125.0
67.00	261.0
68.00	7742.0
69.00	7860.0
70.00	776.0
70.90	172.0
71.90	437.0
73.00	3816.0
74.00	14412.0
75.00	42952.0
76.00	3633.0
77.00	632.0
78.00	418.0
78.90	3449.0
79.90	892.0
80.90	3543.0
82.00	841.0
82.90	160.0
84.30	211.0
85.90	129.0
86.90	2570.0
87.90	2521.0
89.90	115.0
91.00	433.0
91.90	2145.0
92.90	3252.0
94.00	10008.0
95.00	84584.0
96.00	5723.0
97.00	184.0
99.30	110.0
103.70	361.0
104.90	375.0
105.80	433.0
106.70	145.0
109.80	129.0
114.80	103.0
115.80	500.0
116.90	679.0
117.90	516.0
118.80	536.0
127.60	224.0
128.00	324.0
128.80	171.0
129.80	300.0
130.70	138.0
134.80	363.0
136.70	123.0
140.90	930.0
142.90	1218.0
145.40	108.0
147.80	309.0
154.90	220.0
155.70	154.0
158.90	165.0
161.00	176.0
171.20	149.0
171.80	262.0
172.40	362.0
173.00	615.0
173.90	55824.0
174.90	4160.0
175.90	53728.0
176.90	2895.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

178.20177.0

203.90124.0

Instrument :
MSVOA_V

ClientSampleId :
BFB74

m/z	Abundance
36.00	584.0
37.00	3225.0
38.00	3268.0
39.00	1416.0
39.90	888.0
40.90	450.0
42.00	193.0
42.80	293.0
43.90	1399.0
44.90	709.0
46.00	331.0
47.00	626.0
47.90	439.0
49.00	2771.0
50.00	14248.0
51.00	4375.0
52.20	194.0
52.90	258.0
53.80	206.0
55.00	491.0
55.90	1261.0
57.00	2430.0
57.90	278.0
59.90	793.0
60.90	3515.0
62.00	3649.0
63.00	3075.0
64.00	348.0
64.70	114.0
67.00	300.0
68.00	6995.0
69.00	6906.0
70.00	741.0
70.80	173.0
71.80	468.0
73.00	3528.0
74.00	13499.0
75.00	38832.0
76.00	3149.0
77.00	626.0
78.00	519.0
78.90	2997.0
79.90	877.0
80.90	3258.0
82.00	708.0
82.60	170.0
83.00	152.0
84.20	170.0
85.90	123.0
87.00	2434.0
88.00	2521.0
89.90	125.0
90.90	479.0
92.00	1881.0
92.90	3152.0
94.00	9317.0
95.00	78480.0
96.00	4983.0
97.00	164.0
99.30	105.0
103.90	374.0
104.90	345.0
105.80	385.0
106.80	145.0
109.80	117.0
111.70	124.0
113.00	145.0
114.80	112.0
115.80	439.0
116.90	674.0
117.80	484.0
118.80	432.0
127.60	329.0
128.90	175.0
129.70	312.0
130.70	148.0
134.80	309.0
136.60	184.0
140.90	893.0
142.90	1060.0
146.70	104.0
147.80	325.0
154.90	222.0
155.80	131.0
158.80	133.0
160.90	120.0
171.20	166.0
171.90	245.0
172.30	344.0
172.90	617.0
173.90	52040.0
174.90	3884.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

175.90

176.90

178.20

50520.0

2834.0

124.0

Instrument :

MSVOA_V

ClientSampleId :

BFB74

m/z	Abundance
36.70	170.0
37.70	115.0
38.20	219.0
39.20	252.0
40.00	671.0
41.00	330.0
41.90	214.0
43.00	428.0
43.90	678.0
46.00	131.0
49.20	136.0
52.90	173.0
54.00	290.0
54.80	342.0
56.00	304.0
56.90	196.0
60.20	147.0
65.00	111.0
67.00	154.0
67.80	124.0
69.00	243.0
70.00	177.0
72.70	102.0
73.70	112.0
75.00	111.0
75.80	103.0
77.40	108.0
79.00	188.0
80.80	123.0
81.20	137.0
82.30	158.0
82.90	161.0
83.20	175.0
84.10	147.0
84.80	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74