

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
 Data File : VV020811.D
 Acq On : 30 Mar 2021 10:54
 Operator : SY/MD
 Sample : VV0330WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK84

Quant Time: Mar 30 16:06:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 30 04:39:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	643399	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	630124	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	315606	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	185002	40.50	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.00%		
7) Chloroethane-d5	1.571	69	154356	44.70	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.40%		
11) 1,1-Dichloroethene-d2	2.108	63	301868	35.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.06%		
21) 2-Butanone-d5	3.883	46	255924	86.12	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.12%		
24) Chloroform-d	4.349	84	429338	47.29	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.58%		
26) 1,2-Dichloroethane-d4	5.034	65	297412	49.73	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.46%		
32) Benzene-d6	5.050	84	812328	48.36	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.72%		
36) 1,2-Dichloropropane-d6	6.069	67	247469	47.99	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.98%		
41) Toluene-d8	7.317	98	754684	48.27	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.54%		
43) trans-1,3-Dichloroprop...	7.622	79	128216	46.73	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.46%		
47) 2-Hexanone-d5	8.088	63	182506	84.42	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	84.42%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	322597	42.95	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.90%		
64) 1,2-Dichlorobenzene-d4	11.632	152	323242	52.77	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.54%		
Target Compounds					Qvalue	
25) Chloroform	4.378	83	9910	1.16	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020811.D
Acq On : 30 Mar 2021 10:54
Operator : SY/MD
Sample : VV0330WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK84

Quant Time: Mar 30 16:06:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 30 04:39:28 2021
Response via : Initial Calibration

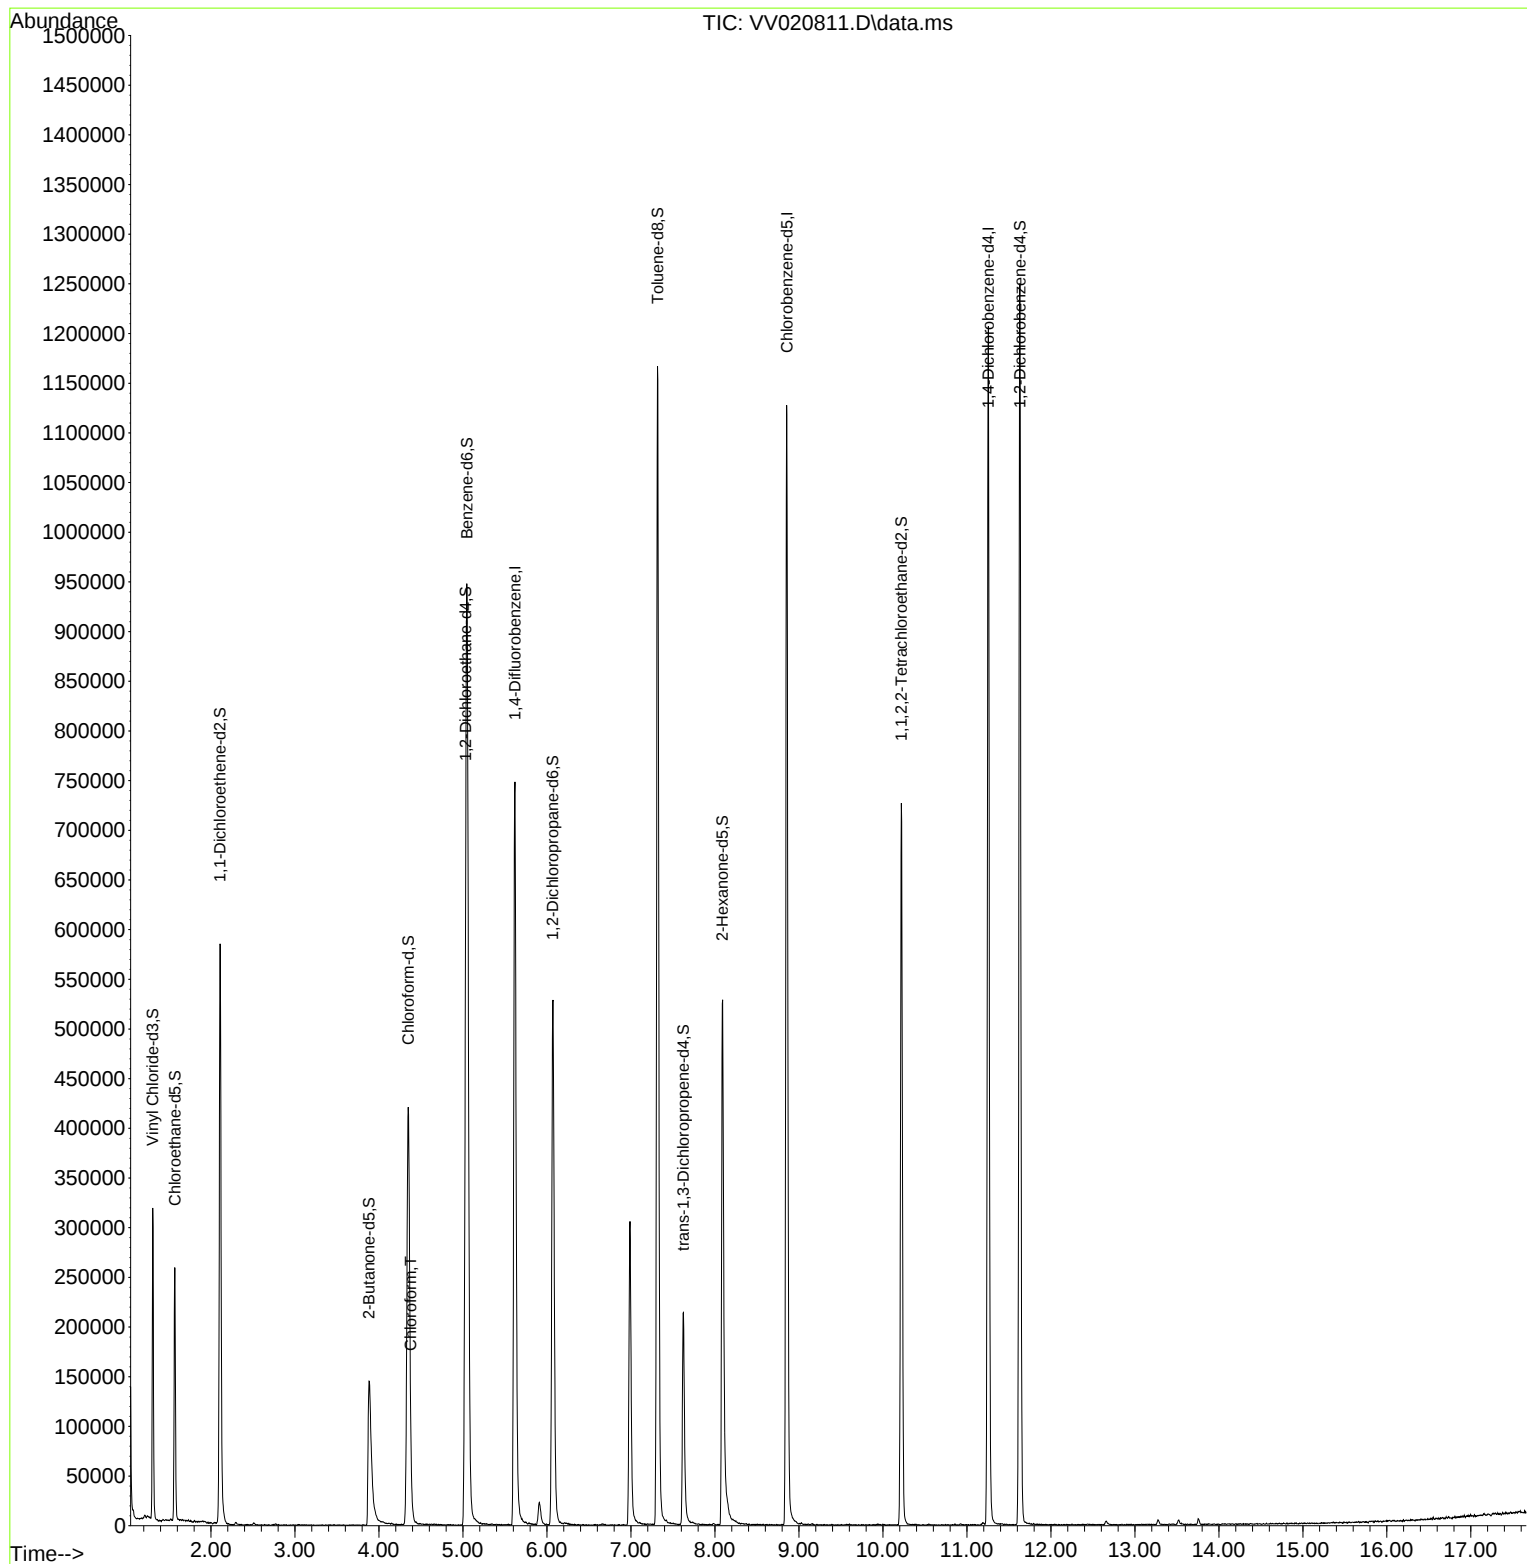

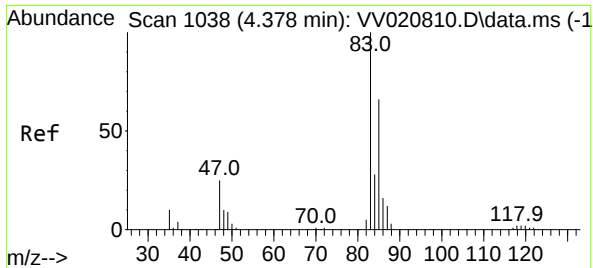

#25
 Chloroform
 Concen: 1.16 ug/L
 RT: 4.378 min Scan# 1038
 Delta R.T. 0.003 min
 Lab File: VV020811.D
 Acq: 30 Mar 2021 10:54

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK84

Tgt Ion: 83 Resp: 9910
 Ion Ratio Lower Upper
 83 100
 85 73.7 46.7 86.7

