

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033021\
 Data File : VW020812.D
 Acq On : 30 Mar 2021 11:37
 Operator : SY/MD
 Sample : M1824-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T3

Quant Time: Mar 30 13:59:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 30 04:39:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	791571	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	774497	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	394591	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	178646	31.79	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	63.58%		
7) Chloroethane-d5	1.568	69	149584	35.21	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	70.42%		
11) 1,1-Dichloroethene-d2	2.108	63	291645	27.51	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.02%#		
21) 2-Butanone-d5	3.876	46	234398	64.11	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	64.11%		
24) Chloroform-d	4.349	84	423051	37.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.74%		
26) 1,2-Dichloroethane-d4	5.031	65	285781	38.84	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.68%		
32) Benzene-d6	5.050	84	794562	38.49	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	76.98%		
36) 1,2-Dichloropropane-d6	6.069	67	236838	37.37	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	74.74%		
41) Toluene-d8	7.317	98	733565	38.17	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	76.34%#		
43) trans-1,3-Dichloroprop...	7.622	79	123589	36.65	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.30%		
47) 2-Hexanone-d5	8.088	63	167868	63.17	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	63.17%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	312465	33.84	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	67.68%		
64) 1,2-Dichlorobenzene-d4	11.632	152	322405	42.10	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.20%		
Target Compounds					Qvalue	
13) Acetone	2.169	43	15807	6.06	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020812.D
Acq On : 30 Mar 2021 11:37
Operator : SY/MD
Sample : M1824-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T3

Quant Time: Mar 30 13:59:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 30 04:39:28 2021
Response via : Initial Calibration

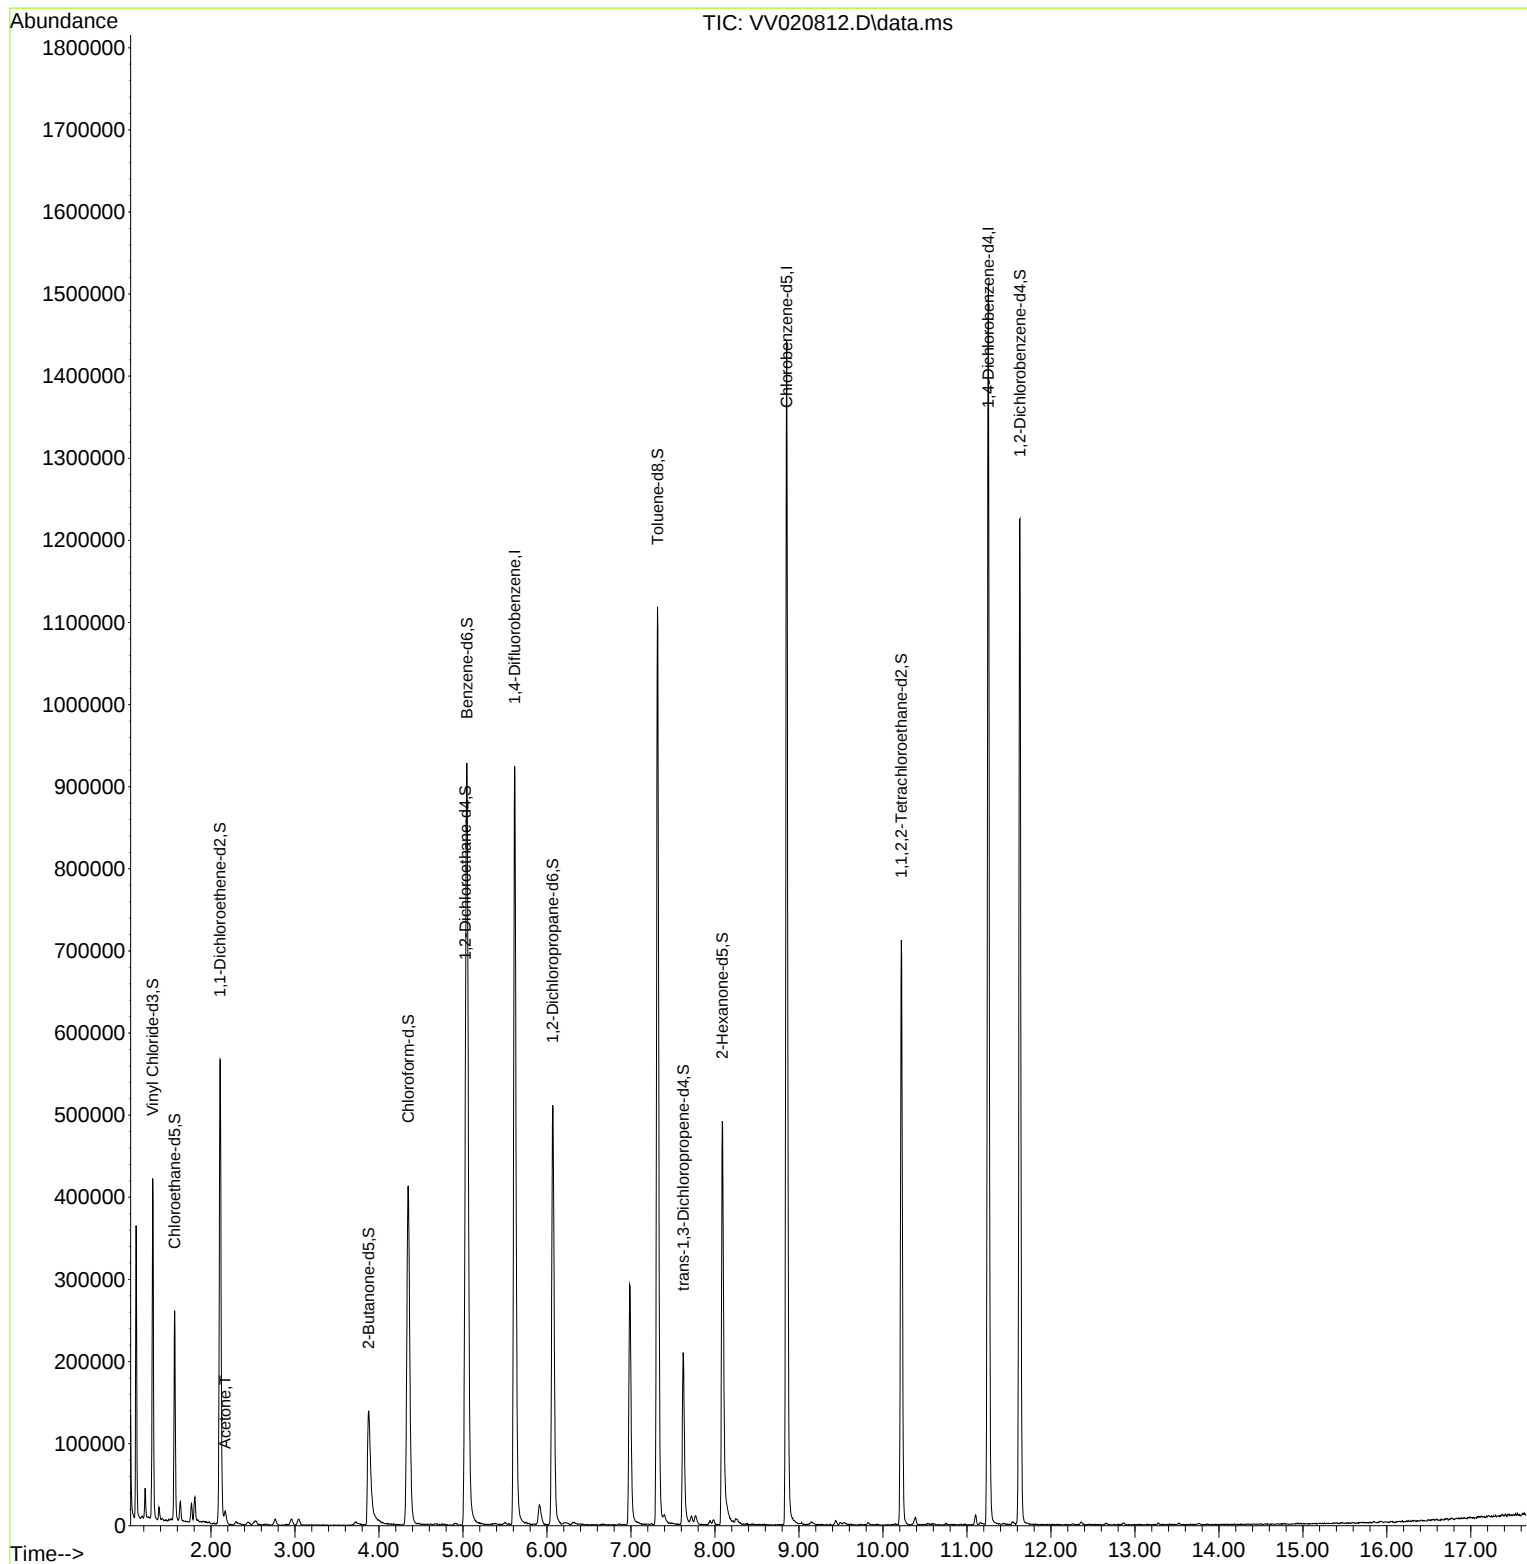

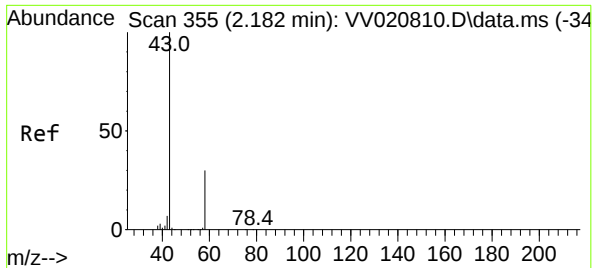

#13
 Acetone
 Concen: 6.06 ug/L
 RT: 2.169 min Scan# 351
 Delta R.T. -0.010 min
 Lab File: VV020812.D
 Acq: 30 Mar 2021 11:37

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T3

Tgt Ion:	43	Resp:	15807
Ion	Ratio	Lower	Upper
43	100		
58	33.6	0.0	60.8

