

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
 Data File : VV020814.D
 Acq On : 30 Mar 2021 12:25
 Operator : SY/MD
 Sample : M1824-15RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W0RE

Quant Time: Mar 30 14:00:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 30 04:39:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	483919	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	480948	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	241013	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	182308	53.07	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	= 106.14%		
7) Chloroethane-d5	1.568	69	153545	59.11	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	= 118.22%		
11) 1,1-Dichloroethene-d2	2.111	63	299427	46.19	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	= 92.38%		
21) 2-Butanone-d5	3.883	46	248855	111.34	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	= 111.34%		
24) Chloroform-d	4.352	84	440134	64.45	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 128.90%#		
26) 1,2-Dichloroethane-d4	5.037	65	300944	66.90	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 133.80%#		
32) Benzene-d6	5.053	84	806709	62.93	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 125.86%#		
36) 1,2-Dichloropropane-d6	6.076	67	243518	61.87	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	= 123.74%#		
41) Toluene-d8	7.320	98	750903	62.93	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	= 125.86%#		
43) trans-1,3-Dichloroprop...	7.625	79	128464	61.35	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	= 122.70%		
47) 2-Hexanone-d5	8.092	63	182101	110.36	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	= 110.36%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	324484	56.60	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	= 113.20%		
64) 1,2-Dichlorobenzene-d4	11.632	152	320575	68.53	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	= 137.06%#		
Target Compounds						
25) Chloroform	4.381	83	7260	1.13	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020814.D
Acq On : 30 Mar 2021 12:25
Operator : SY/MD
Sample : M1824-15RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W0RE

Quant Time: Mar 30 14:00:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 30 04:39:28 2021
Response via : Initial Calibration

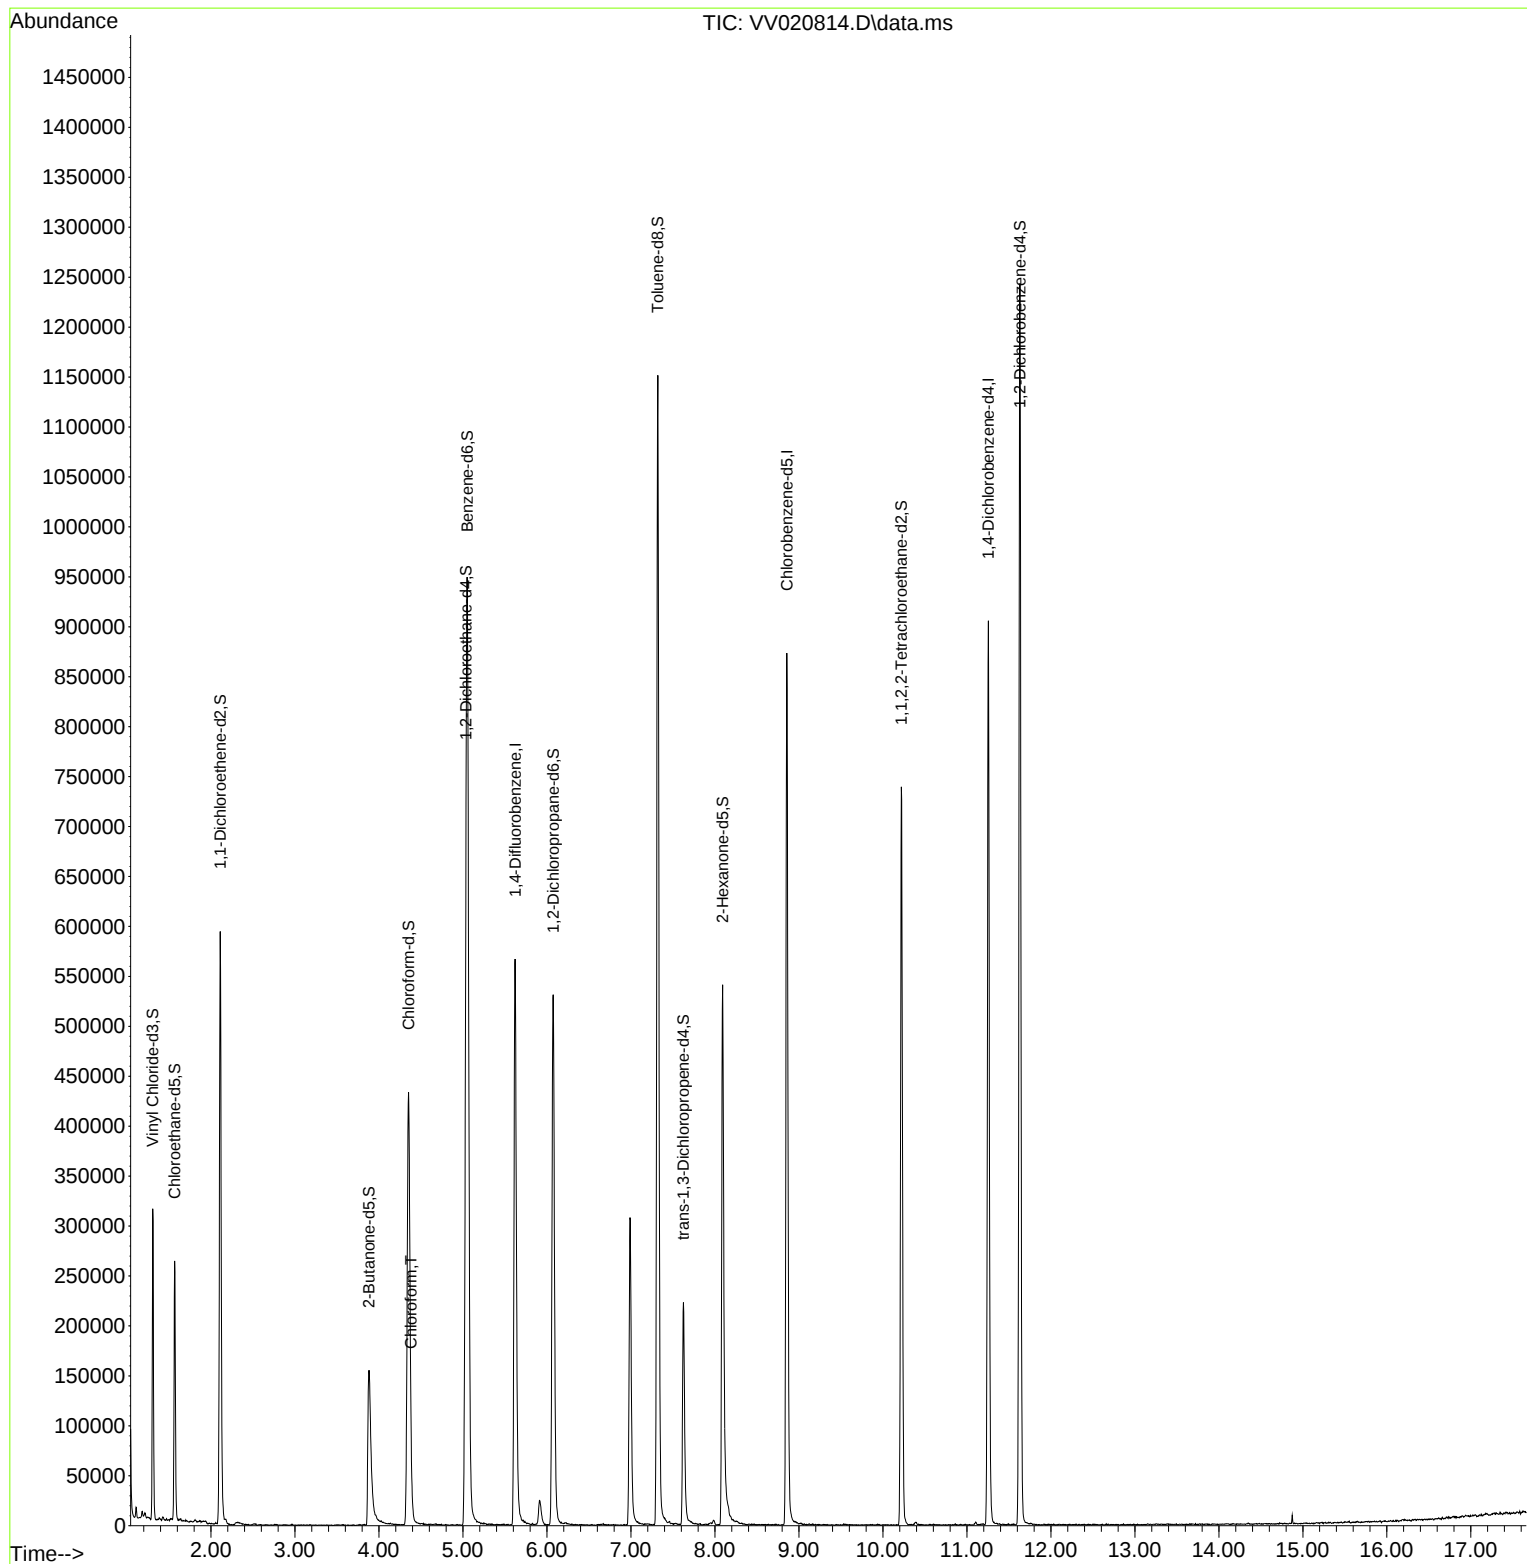

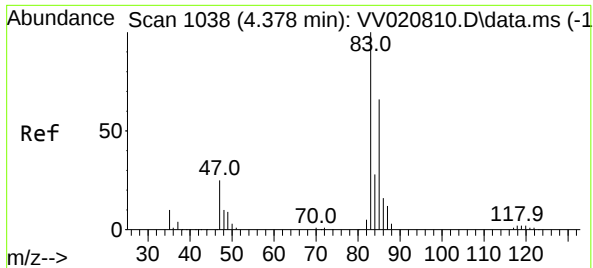

#25
Chloroform
Concen: 1.13 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VV020814.D
Acq: 30 Mar 2021 12:25

Instrument :
MSVOA_V
ClientSampleId :
BG4W0RE

Tgt Ion: 83 Resp: 7260
Ion Ratio Lower Upper
83 100
85 66.0 46.7 86.7

