

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
 Data File : VV020813.D
 Acq On : 30 Mar 2021 12:01
 Operator : SY/MD
 Sample : M1824-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	33	rVB	43228	39643	1.65%	0.212%
2	1.307	77	83	97	rVB	311694	319732	13.28%	1.713%
3	1.568	157	164	178	rVB	251227	287575	11.95%	1.540%
4	2.111	323	333	349	rBV	572971	842591	35.00%	4.513%
5	2.500	452	454	455	rBV	862	339	0.01%	0.002%
6	2.587	476	481	484	rBV2	957	775	0.03%	0.004%
7	2.648	497	500	505	rBV2	442	334	0.01%	0.002%
8	2.748	520	531	533	rBV3	2795	4152	0.17%	0.022%
9	2.844	559	561	563	rVB	426	176	0.01%	0.001%
10	2.880	570	572	574	rBV	433	250	0.01%	0.001%
11	2.957	593	596	598	rBV3	1080	704	0.03%	0.004%
12	3.005	609	611	616	rVB4	704	430	0.02%	0.002%
13	3.053	616	626	631	rBV7	1899	2986	0.12%	0.016%
14	3.095	636	639	644	rVB2	542	385	0.02%	0.002%
15	3.117	644	646	653	rBV3	393	349	0.01%	0.002%
16	3.185	665	667	669	rBV	312	179	0.01%	0.001%
17	3.227	677	680	684	rVB	544	333	0.01%	0.002%
18	3.256	687	689	692	rVB2	335	179	0.01%	0.001%
19	3.275	693	695	697	rBV3	517	228	0.01%	0.001%
20	3.310	704	706	709	rVB	661	352	0.01%	0.002%
21	3.333	710	713	717	rVB2	542	419	0.02%	0.002%
22	3.359	719	721	724	rBV3	370	262	0.01%	0.001%
23	3.433	742	744	746	rBV2	426	192	0.01%	0.001%
24	3.510	765	768	771	rVB2	515	295	0.01%	0.002%
25	3.529	771	774	776	rBV	433	232	0.01%	0.001%
26	3.561	782	784	786	rBV	406	191	0.01%	0.001%
27	3.577	787	789	792	rVV2	405	244	0.01%	0.001%
28	3.593	792	794	796	rVV	556	230	0.01%	0.001%
29	3.619	800	802	805	rVB3	508	211	0.01%	0.001%
30	3.667	814	817	819	rBV2	549	404	0.02%	0.002%
31	3.728	829	836	838	rBV4	1011	1000	0.04%	0.005%
32	3.844	870	872	873	rBV	591	238	0.01%	0.001%
33	3.883	873	884	914	rBV2	150304	407912	16.95%	2.185%
34	4.265	1000	1003	1004	rBV	680	375	0.02%	0.002%
35	4.352	1014	1030	1059	rBV	413496	1029317	42.76%	5.513%
36	4.619	1109	1113	1116	rBV3	1274	1001	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033021\
 Data File : VW020813.D
 Acq On : 30 Mar 2021 12:01
 Operator : SY/MD
 Sample : M1824-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.818	1172	1175	1177	rBV2	902	582	0.02%	0.003%
38	4.924	1204	1208	1209	rBV	590	361	0.01%	0.002%
39	4.979	1220	1225	1228	rBV3	658	704	0.03%	0.004%
40	5.050	1230	1247	1282	rVV2	926712	2407240	100.00%	12.894%
41	5.526	1391	1395	1397	rBV2	727	547	0.02%	0.003%
42	5.622	1412	1425	1449	rBV	761909	1520844	63.18%	8.146%
43	5.818	1483	1486	1490	rBV6	1139	855	0.04%	0.005%
44	5.847	1493	1495	1496	rBV6	948	417	0.02%	0.002%
45	5.912	1506	1515	1534	rVB4	18582	39991	1.66%	0.214%
46	6.072	1551	1565	1597	rBV	520972	1051136	43.67%	5.630%
47	6.522	1699	1705	1709	rVB6	609	686	0.03%	0.004%
48	6.584	1722	1724	1726	rBV2	627	318	0.01%	0.002%
49	6.612	1731	1733	1735	rVB2	837	357	0.01%	0.002%
50	6.638	1735	1741	1742	rBV2	1072	730	0.03%	0.004%
51	6.696	1758	1759	1760	rBV	552	179	0.01%	0.001%
52	6.760	1776	1779	1783	rVB4	880	516	0.02%	0.003%
53	6.796	1786	1790	1792	rBV2	773	695	0.03%	0.004%
54	6.821	1795	1798	1800	rBV2	588	322	0.01%	0.002%
55	6.867	1809	1812	1813	rBV	693	370	0.02%	0.002%
56	6.989	1838	1850	1874	rBV2	297115	544609	22.62%	2.917%
57	7.320	1941	1953	1973	rBV	1129206	1927442	80.07%	10.324%
58	7.625	2038	2048	2072	rBV	214110	377169	15.67%	2.020%
59	7.940	2137	2146	2147	rBV6	2866	3165	0.13%	0.017%
60	8.092	2181	2193	2231	rBV	534856	992136	41.21%	5.314%
61	8.519	2322	2326	2328	rBV3	863	727	0.03%	0.004%
62	8.596	2348	2350	2352	rBV2	658	359	0.01%	0.002%
63	8.661	2368	2370	2373	rBV3	712	459	0.02%	0.002%
64	8.677	2373	2375	2386	rVB5	628	859	0.04%	0.005%
65	8.744	2393	2396	2397	rBV2	467	281	0.01%	0.002%
66	8.780	2405	2407	2411	rVB3	587	399	0.02%	0.002%
67	8.857	2419	2431	2458	rBV	1183117	1911289	79.40%	10.238%
68	9.140	2517	2519	2520	rBV	776	256	0.01%	0.001%
69	9.365	2587	2589	2590	rBV	418	238	0.01%	0.001%
70	9.374	2590	2592	2596	rVB2	987	611	0.03%	0.003%
71	9.397	2596	2599	2602	rBV2	753	469	0.02%	0.003%
72	9.490	2625	2628	2633	rBV5	1410	1680	0.07%	0.009%
73	9.532	2637	2641	2643	rBV2	1481	1332	0.06%	0.007%
74	9.773	2714	2716	2720	rVB4	654	313	0.01%	0.002%
75	9.992	2779	2784	2787	rVB	848	661	0.03%	0.004%
76	10.011	2787	2790	2792	rBV	443	283	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
 Data File : VV020813.D
 Acq On : 30 Mar 2021 12:01
 Operator : SY/MD
 Sample : M1824-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.040	2797	2799	2800	rVB	489	174	0.01%	0.001%
78	10.149	2831	2833	2836	rBV2	553	287	0.01%	0.002%
79	10.223	2844	2856	2876	rBV	713585	1127077	46.82%	6.037%
80	10.394	2902	2909	2916	rVB6	3895	6194	0.26%	0.033%
81	10.622	2978	2980	2982	rBV2	442	222	0.01%	0.001%
82	10.644	2985	2987	2988	rBV	580	234	0.01%	0.001%
83	10.689	2999	3001	3007	rVB	396	322	0.01%	0.002%
84	10.751	3018	3020	3025	rVB2	733	415	0.02%	0.002%
85	10.773	3025	3027	3030	rBV	442	320	0.01%	0.002%
86	10.792	3030	3033	3035	rBV2	706	372	0.02%	0.002%
87	10.921	3069	3073	3078	rBV2	571	600	0.02%	0.003%
88	10.972	3087	3089	3097	rBV4	705	867	0.04%	0.005%
89	11.050	3109	3113	3117	rBV2	998	923	0.04%	0.005%
90	11.101	3123	3129	3140	rVB3	5720	8306	0.35%	0.044%
91	11.162	3140	3148	3150	rBV3	2650	2957	0.12%	0.016%
92	11.255	3165	3177	3196	rBV	1245245	1887215	78.40%	10.109%
93	11.426	3228	3230	3231	rBV	750	295	0.01%	0.002%
94	11.632	3281	3294	3313	rBV	1182600	1884709	78.29%	10.095%
95	11.831	3351	3356	3358	rBV3	928	812	0.03%	0.004%
96	12.056	3423	3426	3428	rBV	570	430	0.02%	0.002%
97	12.156	3455	3457	3460	rVB2	925	436	0.02%	0.002%
98	12.358	3513	3520	3531	rBV7	5591	8715	0.36%	0.047%
99	12.963	3704	3708	3711	rBV3	745	761	0.03%	0.004%
100	13.252	3793	3798	3800	rBV2	1054	924	0.04%	0.005%




Sum of corrected areas: 18669369

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020813.D
Acq On : 30 Mar 2021 12:01
Operator : SY/MD
Sample : M1824-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

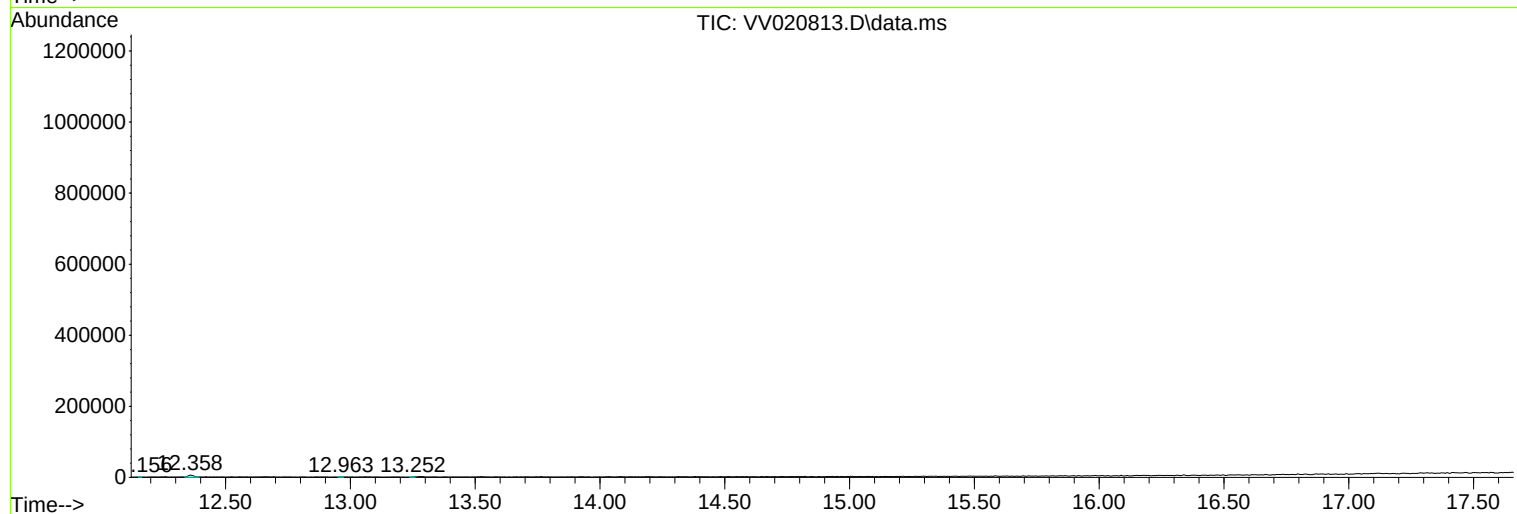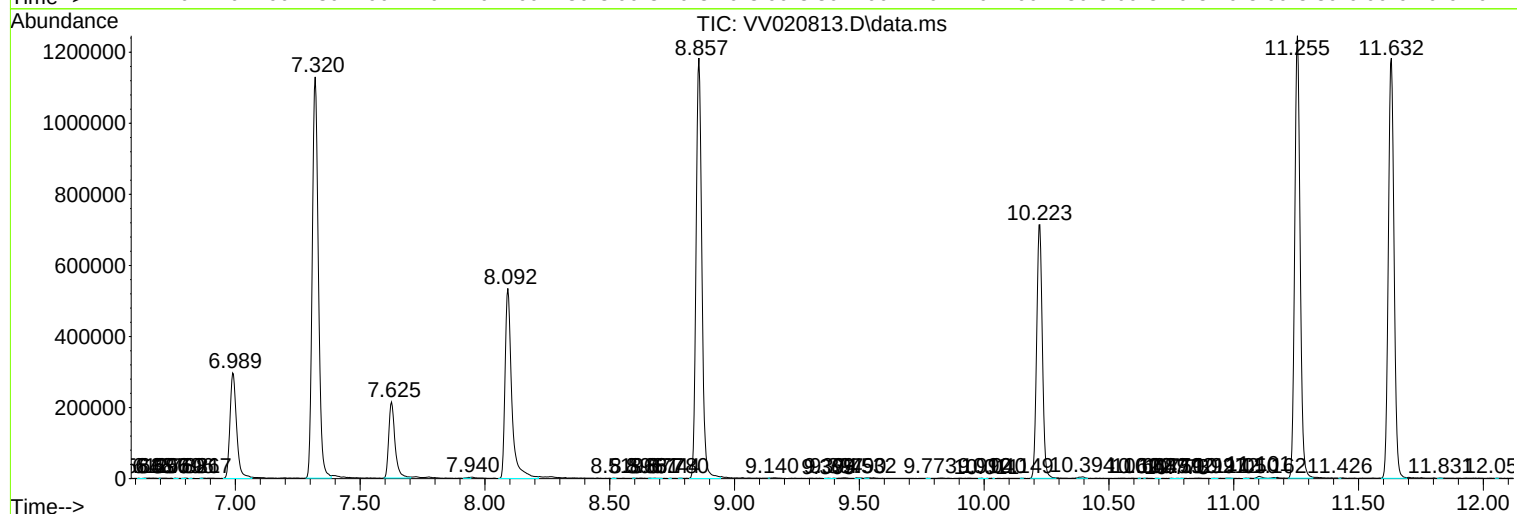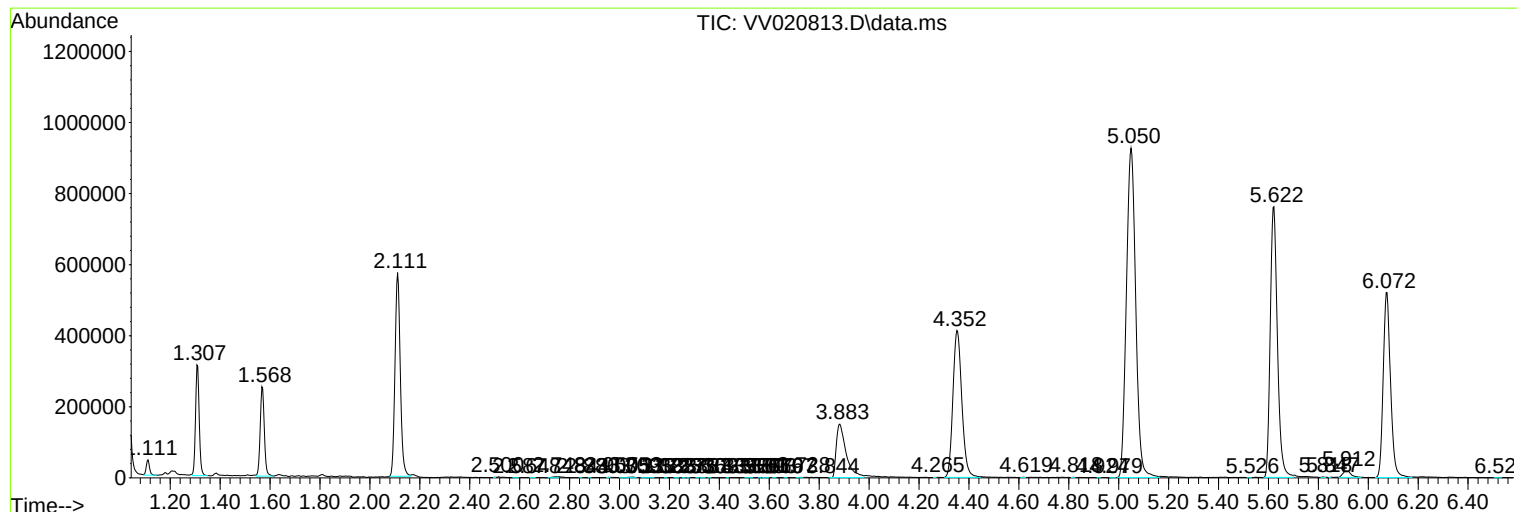

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020813.D
Acq On : 30 Mar 2021 12:01
Operator : SY/MD
Sample : M1824-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020813.D
Acq On : 30 Mar 2021 12:01
Operator : SY/MD
Sample : M1824-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
