

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
 Data File : VV020816.D
 Acq On : 30 Mar 2021 13:36
 Operator : SY/MD
 Sample : M1816-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	294801	292149	12.19%	1.569%
2	1.568	157	164	177	rBV	242633	275811	11.51%	1.481%
3	2.008	299	301	302	rBV2	1560	593	0.02%	0.003%
4	2.111	322	333	361	rVB	568469	852162	35.56%	4.577%
5	2.268	380	382	385	rBV3	581	447	0.02%	0.002%
6	2.429	430	432	434	rVB3	368	144	0.01%	0.001%
7	2.513	448	458	465	rBV6	4564	6843	0.29%	0.037%
8	2.567	472	475	476	rBV	307	138	0.01%	0.001%
9	2.645	497	499	500	rBV	700	286	0.01%	0.002%
10	2.686	510	512	518	rVB3	505	458	0.02%	0.002%
11	2.767	534	537	539	rVB2	566	253	0.01%	0.001%
12	2.863	564	567	570	rVB	339	204	0.01%	0.001%
13	2.879	570	572	574	rBV2	304	207	0.01%	0.001%
14	2.963	593	598	601	rBV2	483	416	0.02%	0.002%
15	3.014	612	614	618	rVB2	658	374	0.02%	0.002%
16	3.053	625	626	628	rBV	263	91	0.00%	0.000%
17	3.066	628	630	633	rBV2	258	151	0.01%	0.001%
18	3.108	642	643	646	rVB	398	117	0.00%	0.001%
19	3.124	646	648	650	rBV	429	224	0.01%	0.001%
20	3.172	658	663	665	rBV	565	394	0.02%	0.002%
21	3.188	665	668	670	rBV	375	243	0.01%	0.001%
22	3.243	679	685	694	rBV4	422	680	0.03%	0.004%
23	3.378	725	727	728	rBV	290	114	0.00%	0.001%
24	3.471	750	756	758	rBV3	399	364	0.02%	0.002%
25	3.526	771	773	775	rVB2	269	71	0.00%	0.000%
26	3.580	788	790	791	rBV	309	138	0.01%	0.001%
27	3.616	800	801	805	rBV	268	146	0.01%	0.001%
28	3.635	805	807	810	rVB2	395	197	0.01%	0.001%
29	3.670	815	818	819	rBV	304	183	0.01%	0.001%
30	3.693	823	825	827	rBV	141	73	0.00%	0.000%
31	3.725	832	835	839	rBV2	374	348	0.01%	0.002%
32	3.764	845	847	850	rVB2	243	152	0.01%	0.001%
33	3.776	850	851	854	rVB2	363	106	0.00%	0.001%
34	3.799	854	858	860	rBV2	523	328	0.01%	0.002%
35	3.828	863	867	872	rBV3	580	599	0.02%	0.003%
36	3.886	875	885	915	rBV	154245	426523	17.80%	2.291%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
 Data File : VV020816.D
 Acq On : 30 Mar 2021 13:36
 Operator : SY/MD
 Sample : M1816-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.352	1012	1030	1060	rBV	416417	1035890	43.22%	5.564%
38	4.799	1166	1169	1173	rBV2	792	596	0.02%	0.003%
39	4.828	1175	1178	1180	rBV3	868	398	0.02%	0.002%
40	4.844	1180	1183	1186	rVV4	877	504	0.02%	0.003%
41	4.892	1196	1198	1200	rBV	724	308	0.01%	0.002%
42	4.969	1219	1222	1227	rBB3	516	425	0.02%	0.002%
43	5.050	1227	1247	1274	rBV2	930778	2396667	100.00%	12.872%
44	5.619	1411	1424	1450	rBV	761194	1522107	63.51%	8.175%
45	5.915	1505	1516	1531	rBV2	22300	46713	1.95%	0.251%
46	6.072	1552	1565	1592	rBV	515240	1045078	43.61%	5.613%
47	6.345	1647	1650	1652	rBV2	624	379	0.02%	0.002%
48	6.452	1681	1683	1686	rVB	564	242	0.01%	0.001%
49	6.490	1692	1695	1696	rBV2	557	240	0.01%	0.001%
50	6.532	1704	1708	1710	rBV3	342	289	0.01%	0.002%
51	6.558	1713	1716	1717	rBV2	437	187	0.01%	0.001%
52	6.574	1717	1721	1723	rBV2	637	352	0.01%	0.002%
53	6.648	1741	1744	1745	rBV2	627	360	0.02%	0.002%
54	6.728	1765	1769	1770	rBV2	510	338	0.01%	0.002%
55	6.763	1778	1780	1785	rVB3	561	459	0.02%	0.002%
56	6.989	1838	1850	1879	rBV	302534	552578	23.06%	2.968%
57	7.320	1940	1953	1976	rBV	1125002	1944319	81.13%	10.443%
58	7.625	2038	2048	2074	rBV	214906	371256	15.49%	1.994%
59	7.898	2131	2133	2136	rBV	625	367	0.02%	0.002%
60	7.927	2140	2142	2143	rBV2	927	360	0.02%	0.002%
61	8.091	2183	2193	2223	rBV	549499	1014715	42.34%	5.450%
62	8.529	2327	2329	2330	rBV	466	219	0.01%	0.001%
63	8.554	2335	2337	2338	rBV2	461	199	0.01%	0.001%
64	8.596	2348	2350	2356	rBV3	927	698	0.03%	0.004%
65	8.660	2368	2370	2374	rBV2	783	510	0.02%	0.003%
66	8.725	2388	2390	2395	rVB3	528	347	0.01%	0.002%
67	8.773	2403	2405	2410	rVB3	792	373	0.02%	0.002%
68	8.857	2418	2431	2454	rBV	1165537	1889040	78.82%	10.146%
69	9.027	2482	2484	2486	rBV2	993	447	0.02%	0.002%
70	9.329	2575	2578	2581	rBV2	972	647	0.03%	0.003%
71	9.535	2637	2642	2645	rBV3	654	611	0.03%	0.003%
72	9.554	2645	2648	2649	rBV	646	262	0.01%	0.001%
73	9.619	2666	2668	2669	rVB	504	147	0.01%	0.001%
74	9.628	2669	2671	2672	rBV	289	96	0.00%	0.001%
75	9.654	2675	2679	2682	rBV3	864	594	0.02%	0.003%
76	9.792	2719	2722	2728	rVB2	968	756	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
 Data File : VV020816.D
 Acq On : 30 Mar 2021 13:36
 Operator : SY/MD
 Sample : M1816-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	9.924	2761	2763	2765	rBV	502	237	0.01%	0.001%
78	10.008	2787	2789	2791	rBV	344	180	0.01%	0.001%
79	10.021	2791	2793	2795	rVB	397	144	0.01%	0.001%
80	10.098	2813	2817	2821	rBV2	412	401	0.02%	0.002%
81	10.220	2842	2855	2874	rBV	718458	1142149	47.66%	6.134%
82	10.477	2933	2935	2937	rBV	389	236	0.01%	0.001%
83	10.545	2954	2956	2959	rBV3	512	427	0.02%	0.002%
84	10.667	2992	2994	2998	rVB	680	424	0.02%	0.002%
85	10.860	3050	3054	3059	rBV3	1076	987	0.04%	0.005%
86	10.982	3090	3092	3095	rBV	398	229	0.01%	0.001%
87	11.255	3165	3177	3197	rBV	1212015	1878359	78.37%	10.089%
88	11.477	3242	3246	3248	rBV3	639	573	0.02%	0.003%
89	11.631	3281	3294	3315	rBV	1222233	1899870	79.27%	10.204%
90	11.956	3393	3395	3397	rBV	692	320	0.01%	0.002%
91	11.975	3397	3401	3403	rBV4	1105	913	0.04%	0.005%
92	12.056	3424	3426	3428	rBV2	545	300	0.01%	0.002%
93	12.545	3575	3578	3581	rBV2	702	504	0.02%	0.003%
94	12.622	3600	3602	3603	rBV	637	226	0.01%	0.001%
95	12.956	3704	3706	3709	rBV2	754	455	0.02%	0.002%




Sum of corrected areas: 18618734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020816.D
Acq On : 30 Mar 2021 13:36
Operator : SY/MD
Sample : M1816-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

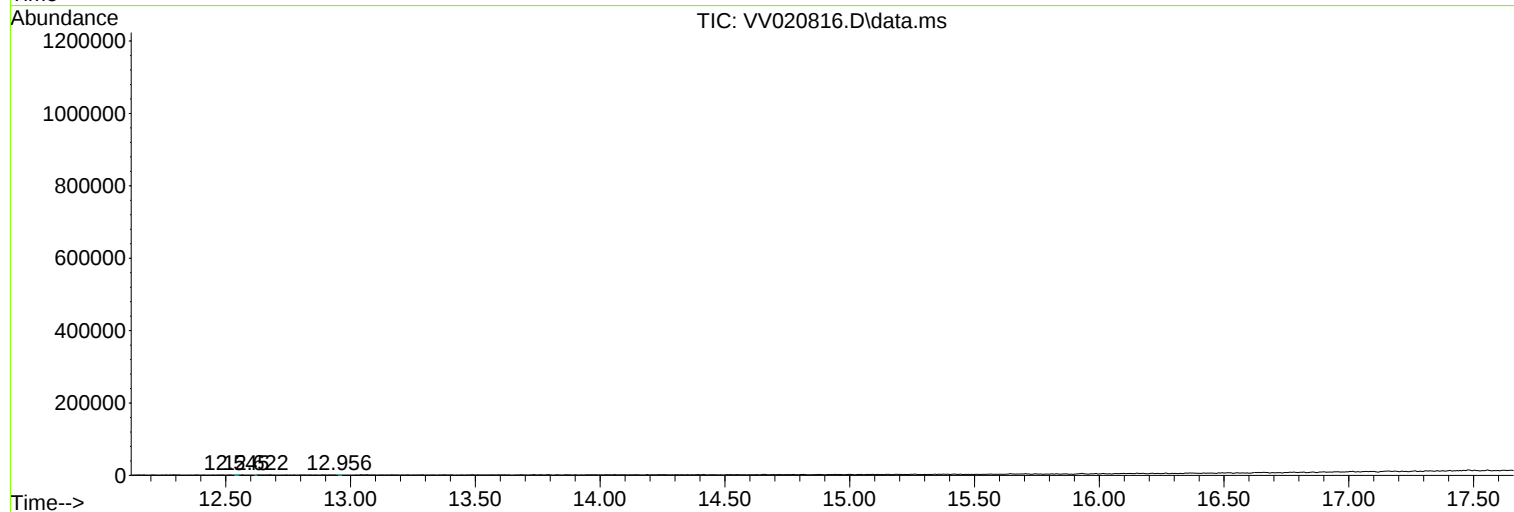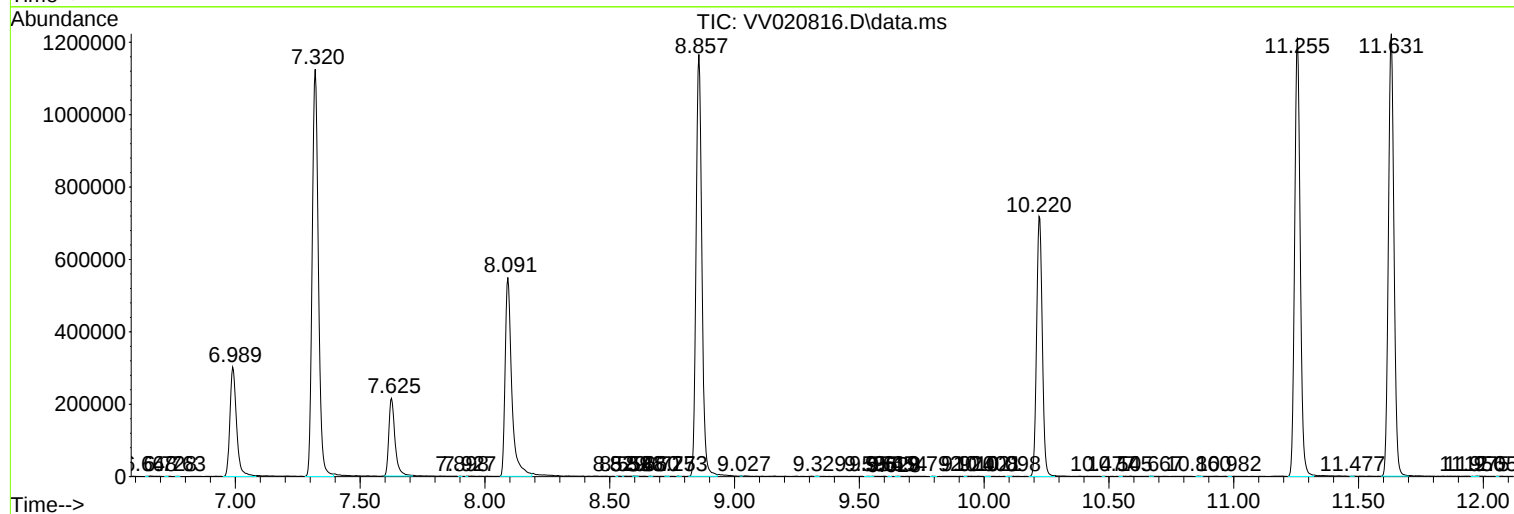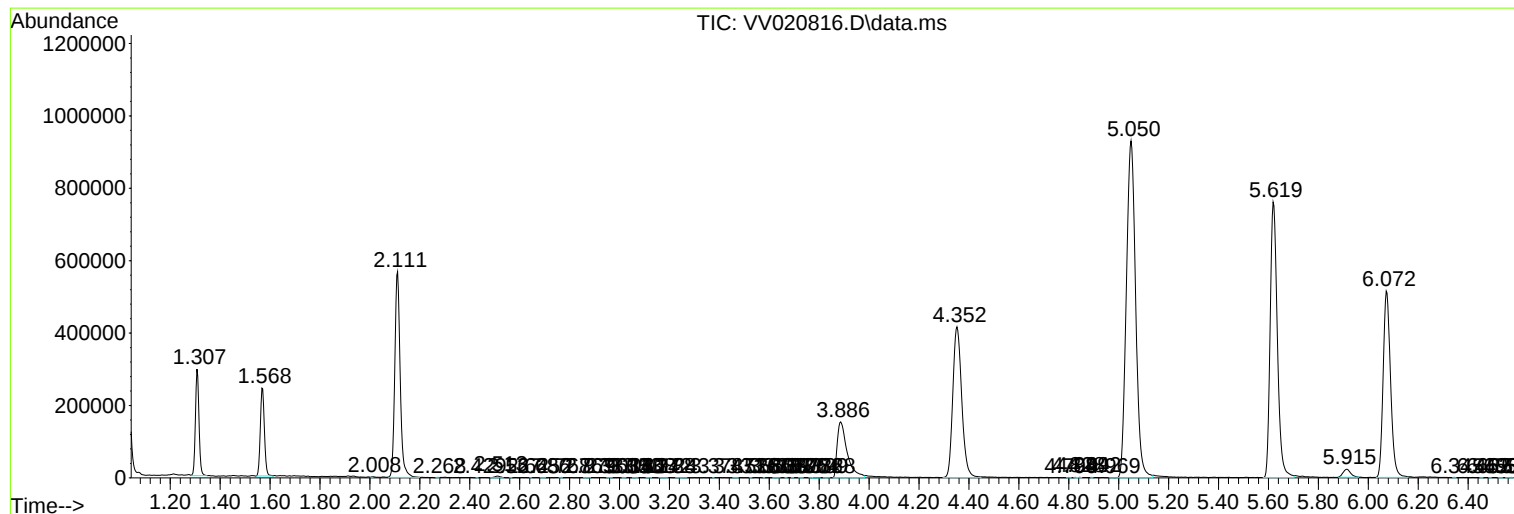

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020816.D
Acq On : 30 Mar 2021 13:36
Operator : SY/MD
Sample : M1816-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020816.D
Acq On : 30 Mar 2021 13:36
Operator : SY/MD
Sample : M1816-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
