
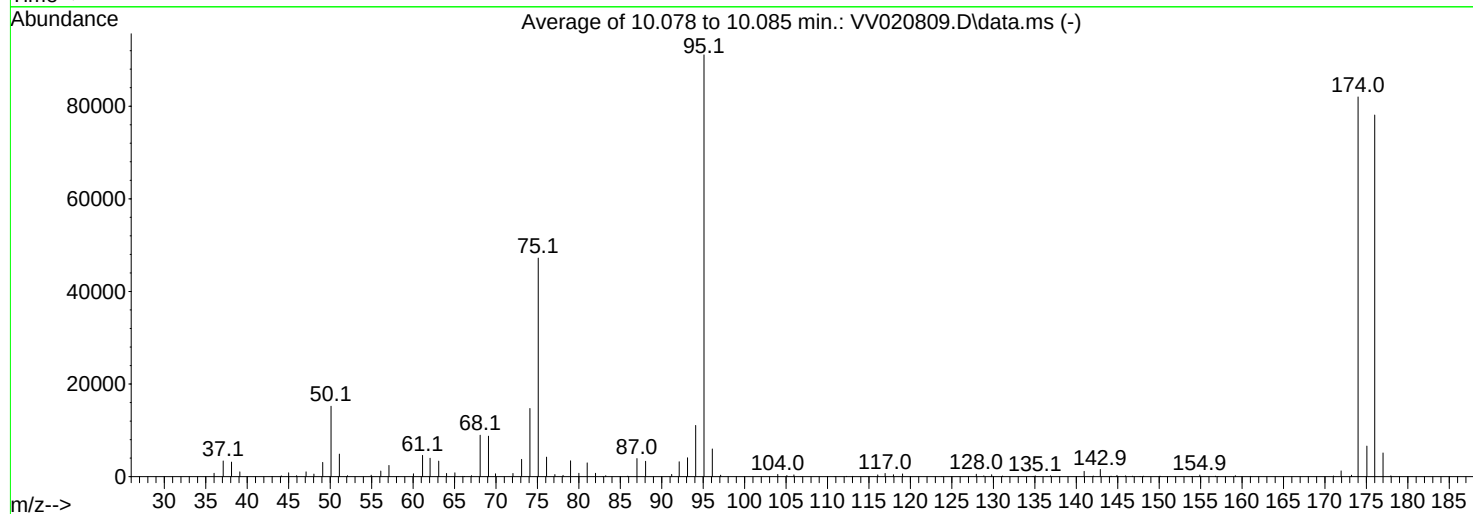


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033021\
Data File : VV020809.D
Acq On : 30 Mar 2021 09:53
Operator : SY/MD
Sample : BFB99
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB99

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis
Last Update : Tue Apr 06 06:22:01 2021

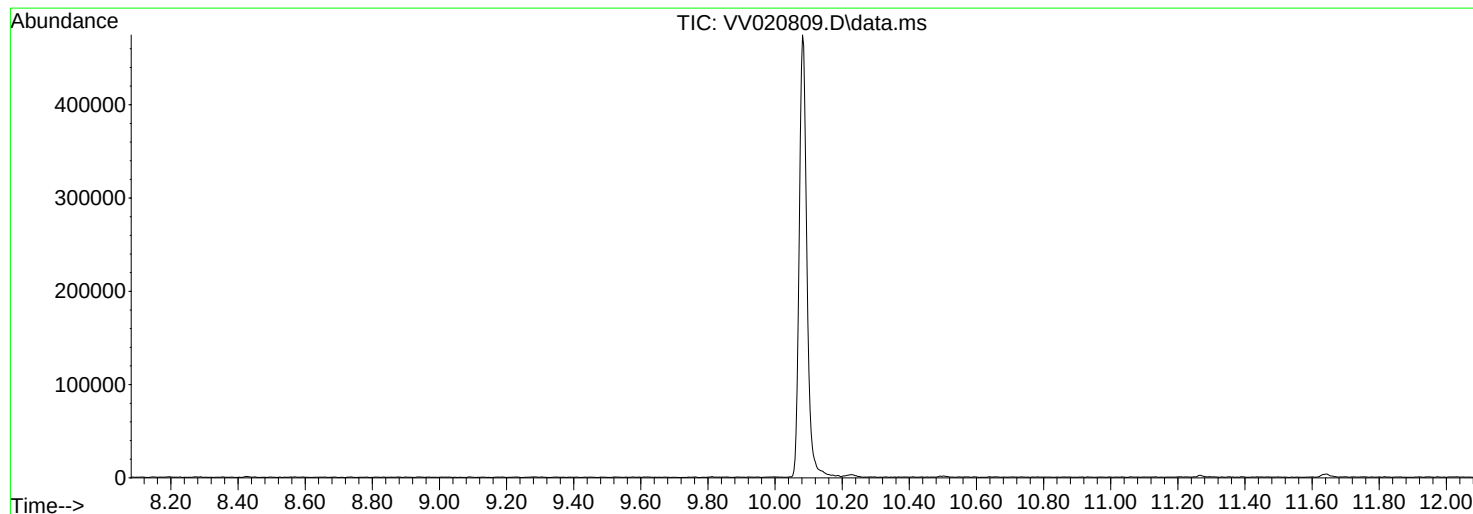

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	15194	PASS
75	95	30	80	51.8	47195	PASS
95	95	100	100	100.0	91099	PASS
96	95	5	9	6.6	5994	PASS
173	174	0.00	2	0.4	315	PASS
174	95	50	120	90.0	82016	PASS
175	174	5	9	8.0	6590	PASS
176	174	95	101	95.2	78091	PASS
177	176	5	9	6.5	5112	PASS

m/z	Abundance
35.70	102.0
39.30	125.0
39.90	277.0
44.20	661.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	762.0
37.10	3183.0
38.10	3137.0
39.10	1240.0
40.00	269.0
44.10	682.0
45.00	880.0
46.00	214.0
47.10	1223.0
48.00	523.0
49.10	3157.0
50.10	15220.0
51.10	4940.0
52.10	164.0
54.90	248.0
56.10	1210.0
57.10	2356.0
60.10	568.0
61.10	4341.0
62.10	3817.0
63.10	3249.0
64.10	783.0
65.10	836.0
66.00	126.0
67.10	202.0
68.10	8700.0
69.10	8241.0
69.90	603.0
72.10	693.0
73.10	3412.0
74.10	14139.0
75.10	45584.0
76.10	3974.0
77.00	478.0
78.00	261.0
79.00	3093.0
80.00	723.0
81.00	3009.0
82.00	752.0
82.90	152.0
83.30	225.0
85.90	177.0
87.00	3821.0
88.10	3096.0
91.20	426.0
92.10	3117.0
93.10	3606.0
94.10	10643.0
95.10	87096.0
96.10	5759.0
97.10	326.0
104.00	573.0
105.00	217.0
106.00	318.0
106.80	124.0
112.30	123.0
113.00	119.0
116.10	318.0
116.90	594.0
118.00	431.0
119.00	493.0
123.80	110.0
128.00	502.0
128.90	190.0
129.80	387.0
131.10	102.0
135.10	290.0
136.90	132.0
140.90	1162.0
142.00	127.0
142.90	1350.0
144.20	190.0
144.90	251.0
146.00	214.0
146.80	134.0
148.10	217.0
154.90	260.0
156.80	204.0
159.20	134.0
172.00	1240.0
173.20	945.0
174.00	76568.0
175.00	6560.0
176.00	73048.0
177.00	4727.0
178.00	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	781.0
37.10	3516.0
38.10	3344.0
39.10	1178.0
40.00	262.0
44.10	843.0
45.00	846.0
46.00	210.0
47.10	1100.0
48.00	581.0
49.10	3116.0
50.10	15491.0
51.10	5035.0
52.10	248.0
54.90	325.0
56.10	1208.0
57.10	2518.0
60.00	646.0
61.20	4797.0
62.10	4190.0
63.10	3435.0
64.10	730.0
65.00	857.0
66.00	121.0
67.00	197.0
68.10	9308.0
69.10	9050.0
69.90	635.0
72.00	753.0
73.10	3875.0
74.10	15180.0
75.10	48912.0
76.10	4256.0
77.10	444.0
78.10	259.0
79.00	3595.0
80.00	764.0
81.00	3006.0
82.00	806.0
83.20	233.0
85.90	129.0
87.00	4030.0
88.10	3451.0
91.20	526.0
92.10	3437.0
93.10	4169.0
94.10	11478.0
95.10	94664.0
96.10	6184.0
97.10	315.0
104.00	483.0
105.10	253.0
106.00	385.0
112.30	103.0
113.10	111.0
116.10	390.0
116.90	702.0
118.00	454.0
119.10	631.0
127.90	566.0
128.90	205.0
129.80	438.0
131.10	175.0
135.00	227.0
136.90	178.0
141.00	1160.0
142.10	134.0
142.90	1645.0
144.20	116.0
144.90	260.0
145.90	194.0
146.80	130.0
147.70	120.0
148.10	150.0
150.10	156.0
153.90	104.0
154.90	388.0
156.80	148.0
159.20	231.0
161.10	124.0
171.10	229.0
172.00	1261.0
174.00	84864.0
175.00	6956.0
176.00	80648.0
177.00	5237.0
178.00	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	693.0
37.10	3493.0
38.10	2953.0
39.10	1096.0
40.00	264.0
43.00	123.0
44.00	1011.0
45.00	757.0
45.90	165.0
47.10	819.0
48.10	565.0
49.10	2951.0
50.10	14872.0
51.10	4666.0
52.10	269.0
55.00	368.0
56.10	1218.0
57.10	2354.0
58.20	129.0
60.10	694.0
61.20	4644.0
62.00	3894.0
63.10	3416.0
64.00	601.0
65.10	803.0
66.20	105.0
67.00	191.0
68.10	8815.0
69.10	8969.0
70.00	622.0
72.00	630.0
73.10	3888.0
74.10	14822.0
75.10	47088.0
76.10	4373.0
77.20	457.0
78.20	307.0
79.00	3581.0
80.00	720.0
81.00	2883.0
82.00	661.0
83.20	171.0
87.00	3888.0
88.00	3420.0
91.20	552.0
92.10	3116.0
93.10	4452.0
94.10	11046.0
95.10	91536.0
96.10	6039.0
97.10	259.0
104.00	378.0
105.20	243.0
105.90	439.0
110.90	106.0
116.00	471.0
117.00	744.0
117.90	406.0
119.10	671.0
127.90	463.0
128.80	177.0
129.80	481.0
131.10	181.0
134.80	191.0
136.90	199.0
141.00	1087.0
142.10	204.0
142.90	1650.0
144.90	295.0
145.90	133.0
150.10	169.0
154.90	369.0
157.10	161.0
159.20	279.0
161.00	131.0
171.00	195.0
171.90	1192.0
174.00	84616.0
175.10	6253.0
176.00	80576.0
177.00	5371.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99