

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030356.D
 Acq On : 30 Mar 2023 13:59
 Operator : SY/MD
 Sample : 02132-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMA6

Quant Time: Mar 31 05:40:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	157609	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	152813	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	71394	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	33589	3.218	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	64.400%	
7) Chloroethane-d5	1.539	69	37698	3.721	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	74.400%	
11) 1,1-Dichloroethene-d2	2.063	63	59949	2.420	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	48.400%#	
20) 2-Butanone-d5	3.818	46	113662	42.128	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	84.260%	
24) Chloroform-d	4.262	84	100994	3.997	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.000%	
26) 1,2-Dichloroethane-d4	4.953	65	51288	4.303	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.000%	
32) Benzene-d6	4.970	84	172133	3.997	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.000%	
36) 1,2-Dichloropropane-d6	5.998	67	56696	4.205	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	84.200%	
41) Toluene-d8	7.252	98	141367	3.575	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	71.400%	
43) trans-1,3-Dichloroprop...	7.561	79	18699	3.684	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	73.600%	
46) 2-Hexanone-d5	8.034	63	83515	40.946	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	81.900%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	41711	3.926	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	78.600%	
66) 1,2-Dichlorobenzene-d4	11.571	152	58062	4.550	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	91.000%	
Target Compounds						
					Qvalue	
13) Acetone	2.150	43	5487	2.127	ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030356.D
Acq On : 30 Mar 2023 13:59
Operator : SY/MD
Sample : 02132-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMA6

Quant Time: Mar 31 05:40:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration

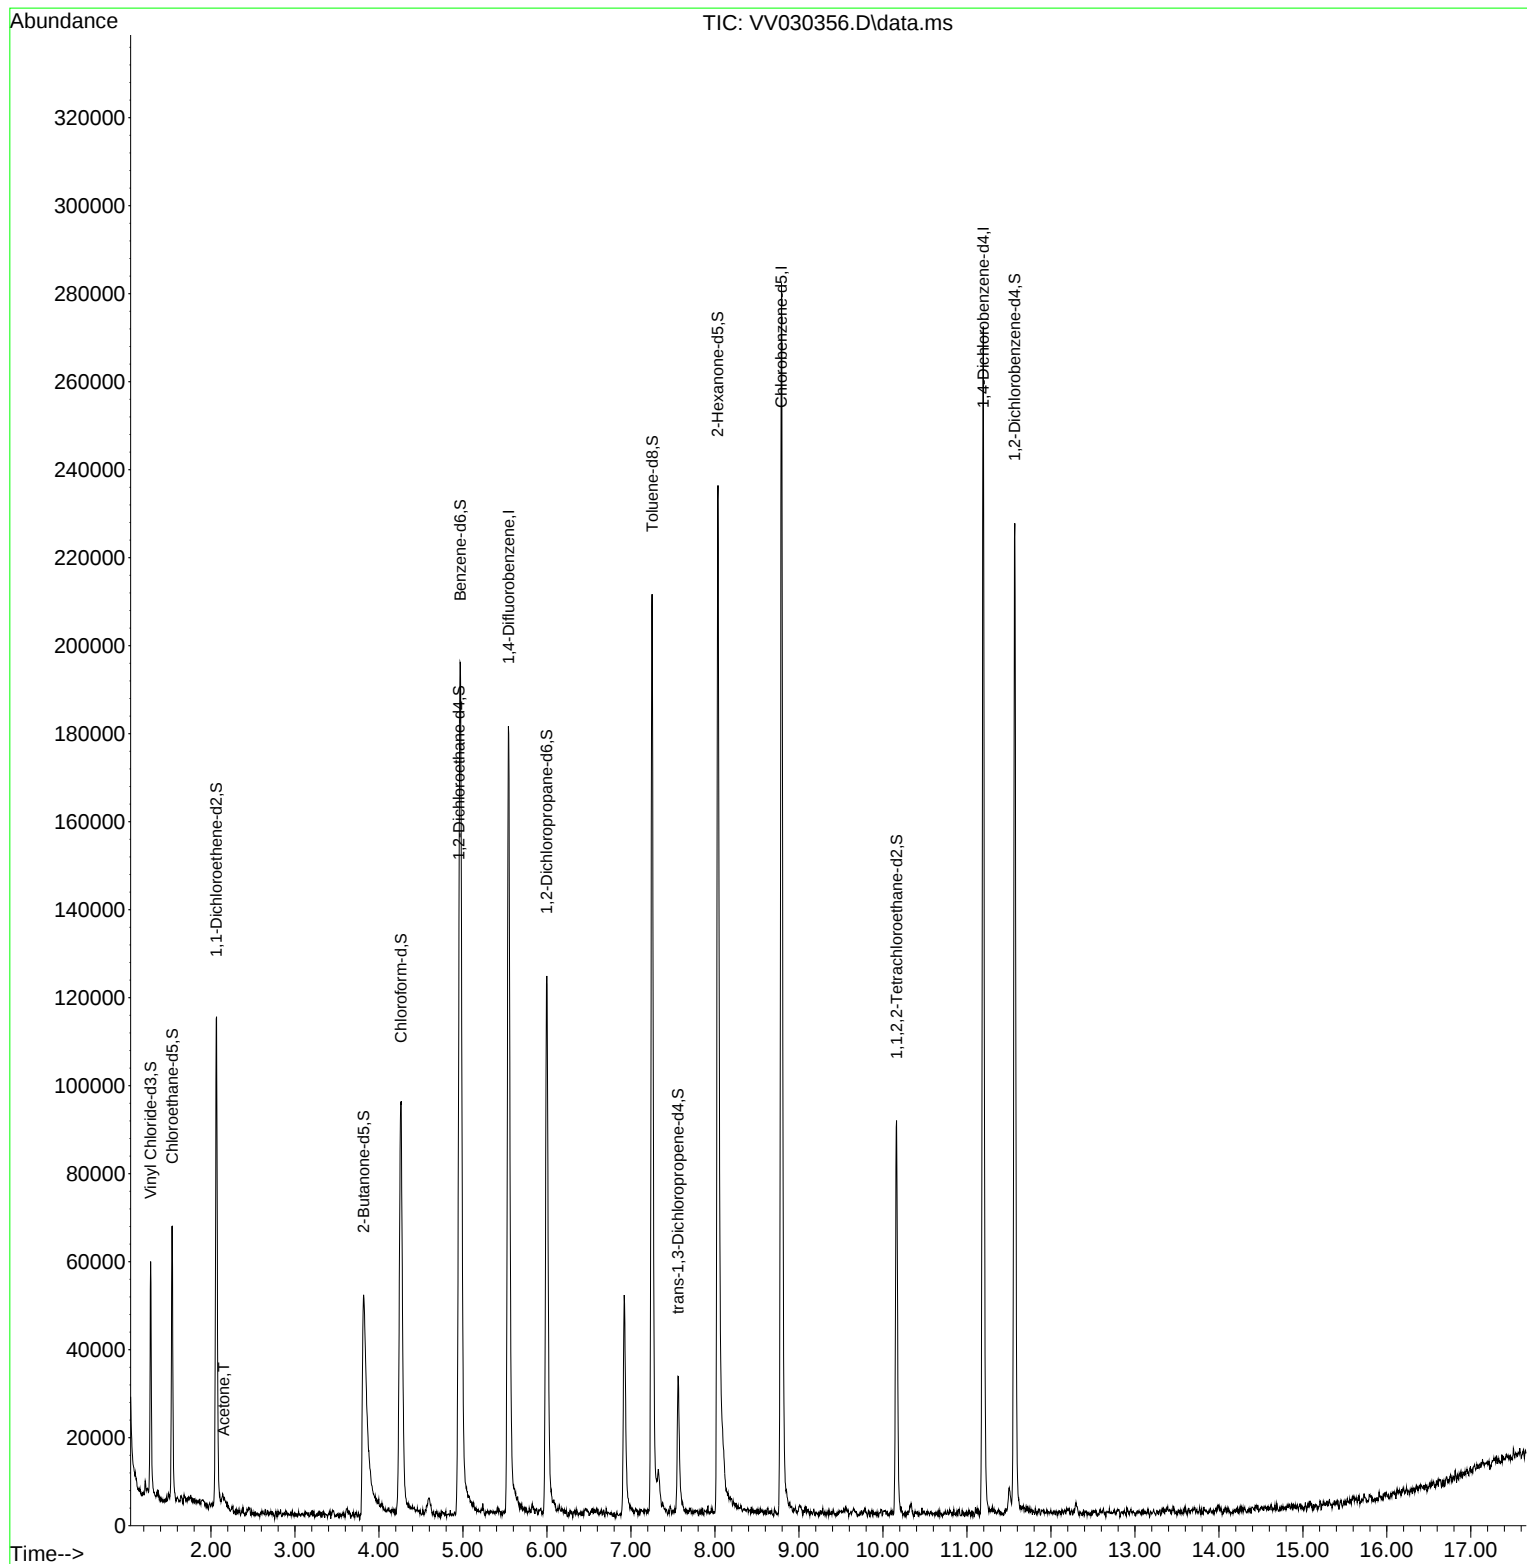

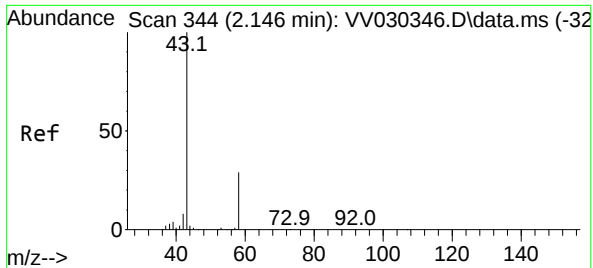

#13
 Acetone
 Concen: 2.127 ug/L
 RT: 2.150 min Scan# 34
 Delta R.T. 0.003 min
 Lab File: VV030356.D
 Acq: 30 Mar 2023 13:59

Instrument :
 MSVOA_V
 ClientSampleId :
 COMA6

Tgt Ion: 43 Resp: 5487

Ion	Ratio	Lower	Upper
43	100		
58	12.1	0.0	40.8

