

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030348.D
 Acq On : 30 Mar 2023 10:45
 Operator : SY/MD
 Sample : 02099-01DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	12	14	23	rVB3	10860	11251	1.07%	0.185%
2	1.281	66	75	84	rBV	62075	68937	6.56%	1.133%
3	1.535	148	154	166	rVB	67082	78218	7.44%	1.286%
4	2.066	306	319	334	rBV	126726	184996	17.60%	3.041%
5	2.455	428	440	454	rBV2	19082	36709	3.49%	0.604%
6	2.712	503	520	547	rBV	220036	486262	46.27%	7.995%
7	3.825	851	866	899	rBV2	54898	238576	22.70%	3.922%
8	4.259	980	1001	1024	rBV2	106519	275760	26.24%	4.534%
9	4.969	1205	1222	1252	rBV2	211633	563735	53.65%	9.268%
10	5.545	1385	1401	1426	rBV	152125	330963	31.49%	5.441%
11	5.998	1526	1542	1564	rBV	134190	286940	27.31%	4.718%
12	6.921	1819	1829	1849	rBV2	54205	110069	10.47%	1.810%
13	7.252	1920	1932	1949	rBV	233170	418511	39.83%	6.881%
14	7.329	1952	1956	1968	rVB7	8231	14184	1.35%	0.233%
15	7.561	2019	2028	2045	rBV2	33922	63503	6.04%	1.044%
16	7.911	2118	2137	2156	rBV	618214	1050846	100.00%	17.277%
17	8.037	2165	2176	2208	rBV	265458	537610	51.16%	8.839%
18	8.792	2400	2411	2428	rBV	236368	399679	38.03%	6.571%
19	10.162	2826	2837	2850	rBV	101298	160239	15.25%	2.634%
20	11.194	3147	3158	3179	rBV	236248	376867	35.86%	6.196%
21	11.570	3262	3275	3294	rVB	236453	388560	36.98%	6.388%




Sum of corrected areas: 6082415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030348.D
Acq On : 30 Mar 2023 10:45
Operator : SY/MD
Sample : 02099-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

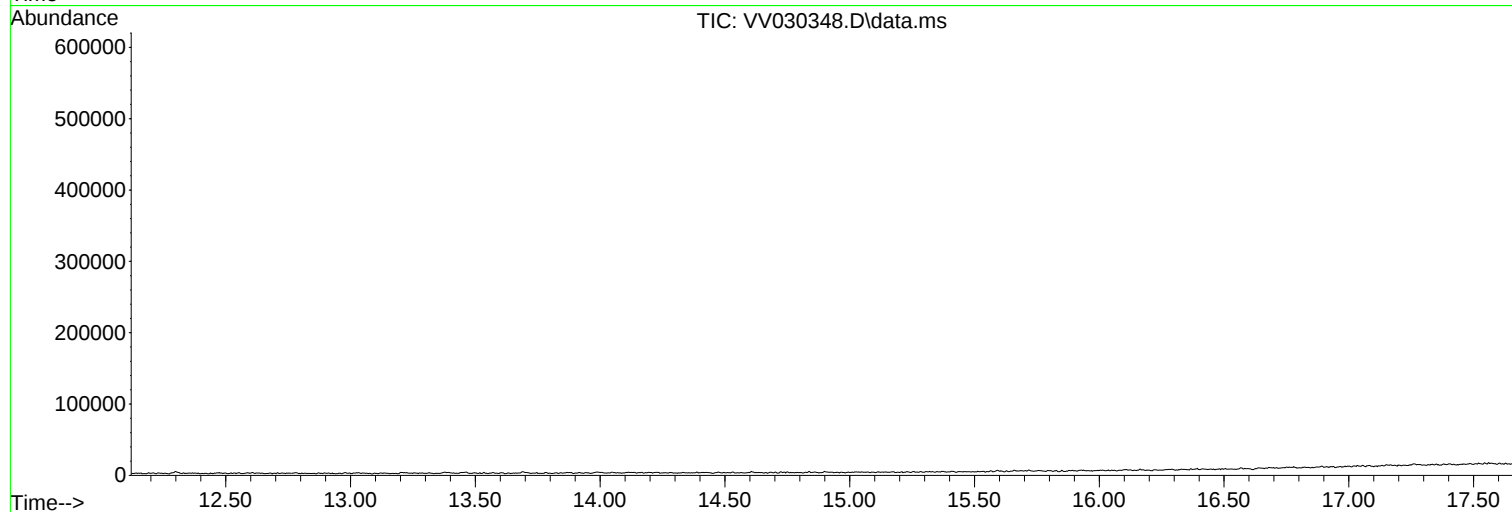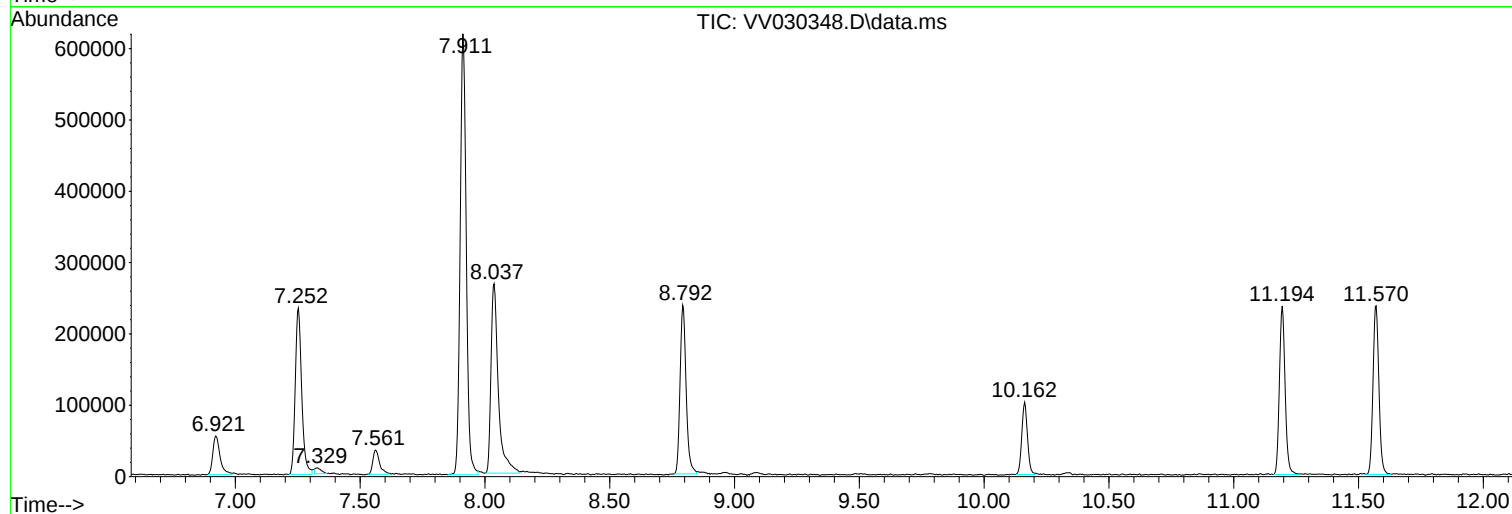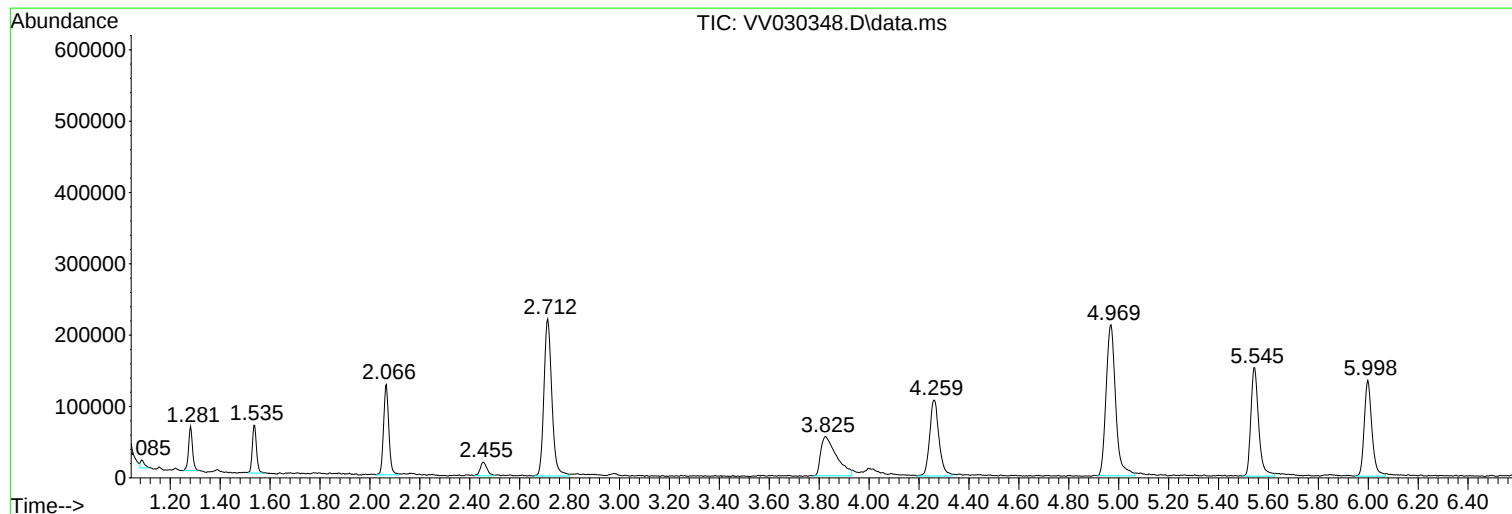

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030348.D
Acq On : 30 Mar 2023 10:45
Operator : SY/MD
Sample : 02099-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030348.D
Acq On : 30 Mar 2023 10:45
Operator : SY/MD
Sample : 02099-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc