

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030350.D
 Acq On : 30 Mar 2023 11:33
 Operator : SY/MD
 Sample : 02099-02DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	66	75	84	rBV	56112	62826	11.77%	1.302%
2	1.539	147	155	164	rVB	64107	75296	14.10%	1.560%
3	2.063	307	318	333	rBV	114857	173472	32.49%	3.594%
4	2.455	430	440	453	rVB	17799	30860	5.78%	0.639%
5	2.712	499	520	539	rBV	170853	368426	68.99%	7.633%
6	3.815	851	863	895	rBV	55518	201231	37.68%	4.169%
7	4.259	982	1001	1023	rBV2	97534	254467	47.65%	5.272%
8	4.966	1201	1221	1242	rBV2	206127	534001	100.00%	11.064%
9	5.542	1385	1400	1428	rBV	160437	352043	65.93%	7.294%
10	5.998	1527	1542	1560	rBV	130070	273362	51.19%	5.664%
11	6.921	1818	1829	1848	rBV	52790	107496	20.13%	2.227%
12	7.252	1921	1932	1952	rBV	222789	402327	75.34%	8.336%
13	7.561	2018	2028	2044	rBV	32359	61637	11.54%	1.277%
14	7.915	2124	2138	2154	rBV2	41265	74077	13.87%	1.535%
15	8.034	2164	2175	2210	rBV	251787	510174	95.54%	10.570%
16	8.792	2397	2411	2432	rBV	244344	418286	78.33%	8.666%
17	10.162	2822	2837	2854	rBV	97899	158887	29.75%	3.292%
18	11.194	3146	3158	3178	rBV	244020	389785	72.99%	8.076%
19	11.570	3263	3275	3293	rBV	234155	377979	70.78%	7.831%




Sum of corrected areas: 4826632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030350.D
Acq On : 30 Mar 2023 11:33
Operator : SY/MD
Sample : 02099-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

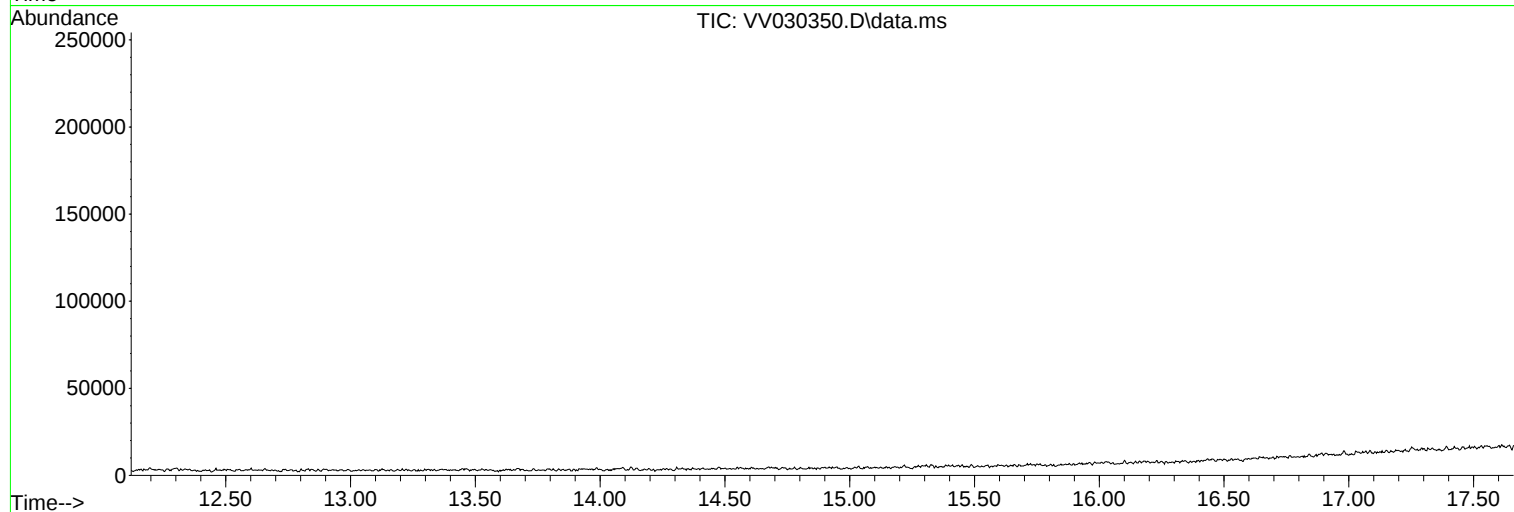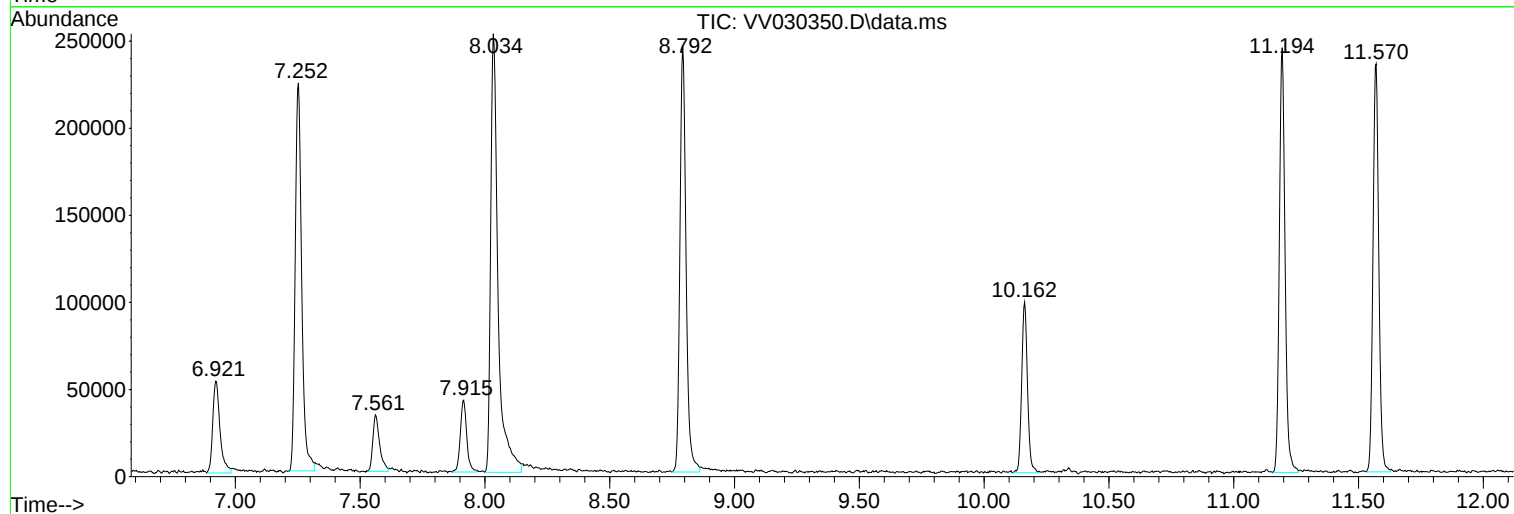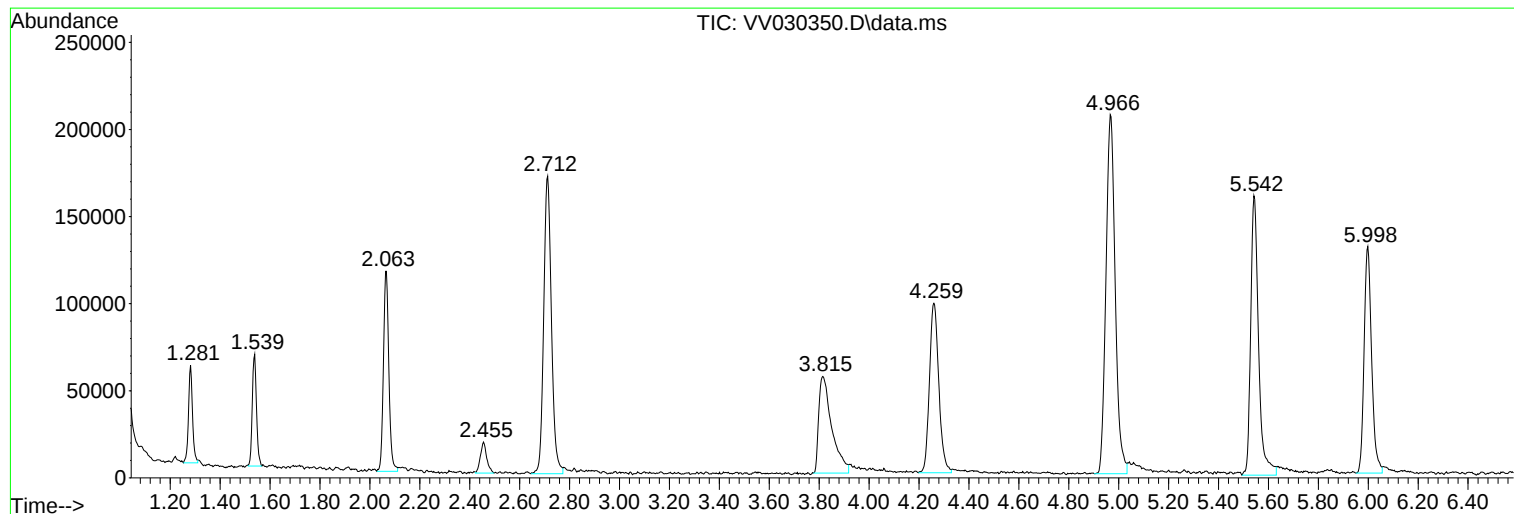

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030350.D
Acq On : 30 Mar 2023 11:33
Operator : SY/MD
Sample : 02099-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030350.D
Acq On : 30 Mar 2023 11:33
Operator : SY/MD
Sample : 02099-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc