

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030351.D
 Acq On : 30 Mar 2023 11:58
 Operator : SY/MD
 Sample : 02099-04DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	91	rVB	68958	77319	12.98%	1.362%
2	1.535	147	154	166	rBV	71714	83592	14.04%	1.472%
3	2.066	307	319	331	rBV	130607	194380	32.64%	3.423%
4	2.455	429	440	453	rBV2	19253	34924	5.86%	0.615%
5	2.712	501	520	545	rBV	185786	403269	67.72%	7.102%
6	3.815	850	863	894	rBV	62712	234487	39.38%	4.130%
7	4.259	986	1001	1024	rBV	108680	283137	47.55%	4.987%
8	4.969	1201	1222	1238	rBV3	233700	595496	100.00%	10.488%
9	5.053	1240	1248	1268	rVB2	29947	74624	12.53%	1.314%
10	5.542	1387	1400	1422	rBV	197145	418305	70.24%	7.367%
11	5.998	1528	1542	1561	rBV	143917	308136	51.74%	5.427%
12	6.921	1817	1829	1846	rBV2	62634	117403	19.72%	2.068%
13	7.252	1919	1932	1950	rBV	253491	461336	77.47%	8.125%
14	7.561	2017	2028	2050	rBV2	37320	72637	12.20%	1.279%
15	7.915	2125	2138	2151	rBV2	84600	147953	24.85%	2.606%
16	8.034	2164	2175	2201	rBV	279246	564825	94.85%	9.948%
17	8.792	2398	2411	2433	rBV	303067	517630	86.92%	9.117%
18	10.162	2826	2837	2853	rBV	106417	173711	29.17%	3.059%
19	11.194	3143	3158	3176	rBV	303696	482727	81.06%	8.502%
20	11.570	3263	3275	3294	rBV	262860	431981	72.54%	7.608%




Sum of corrected areas: 5677872

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030351.D
Acq On : 30 Mar 2023 11:58
Operator : SY/MD
Sample : 02099-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

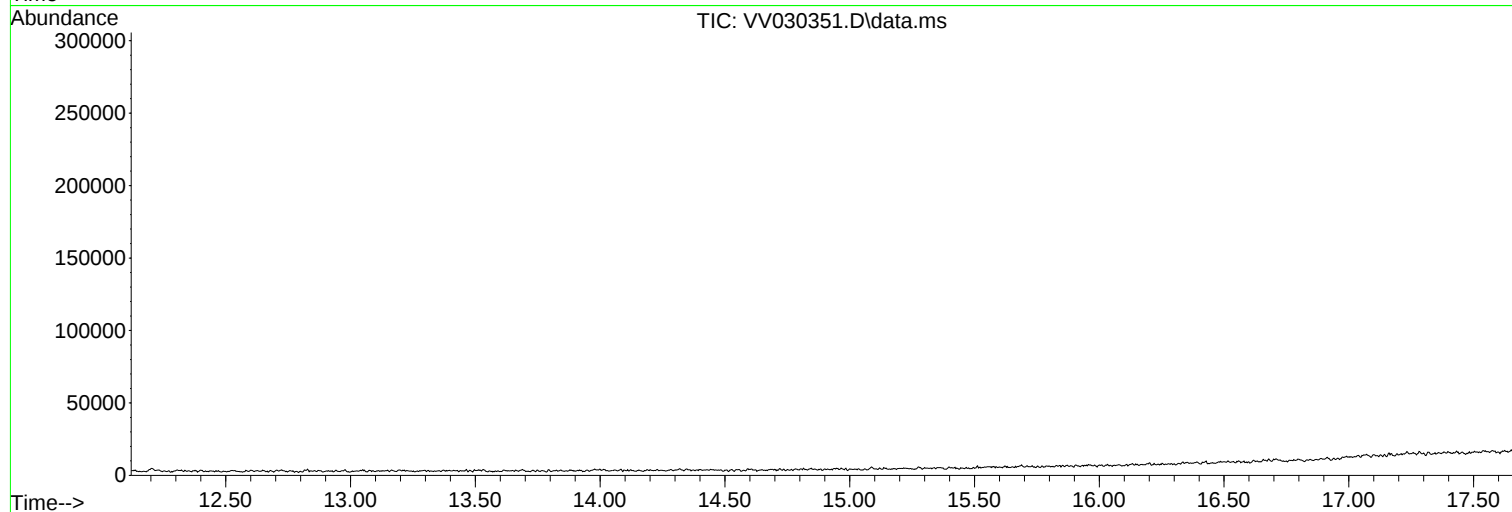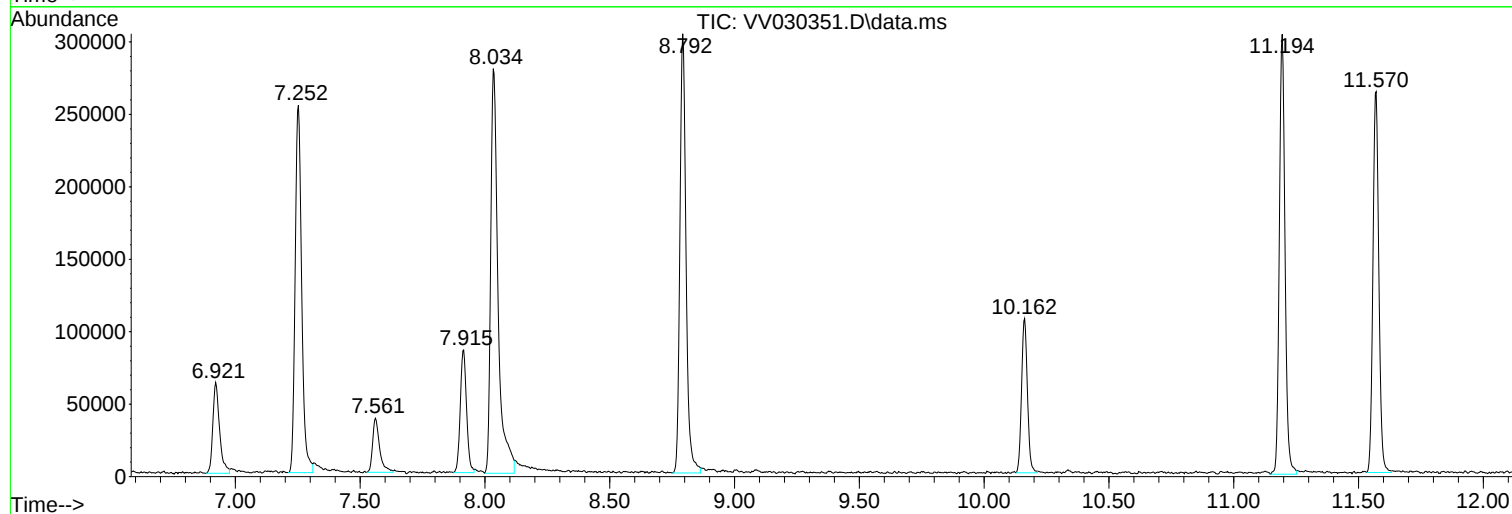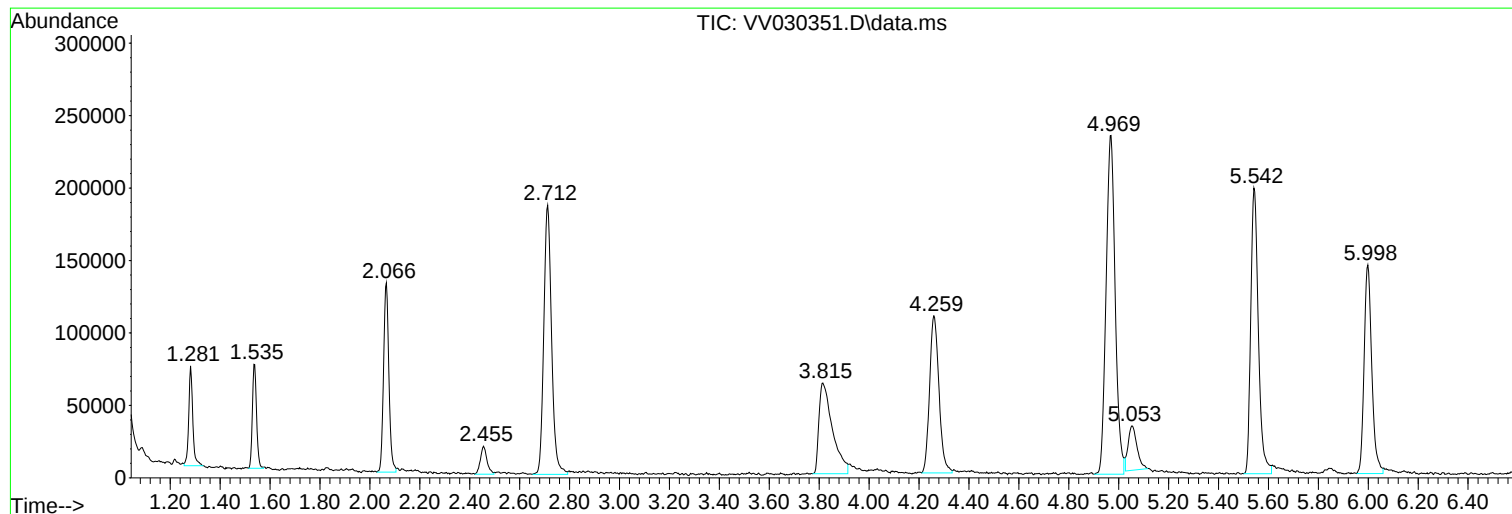

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030351.D
Acq On : 30 Mar 2023 11:58
Operator : SY/MD
Sample : 02099-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030351.D
Acq On : 30 Mar 2023 11:58
Operator : SY/MD
Sample : 02099-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc