

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030352.D
 Acq On : 30 Mar 2023 12:21
 Operator : SY/MD
 Sample : 02092-19 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB991

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rVB	60288	67000	11.31%	1.432%
2	1.532	147	153	164	rVB	70755	80142	13.53%	1.713%
3	2.060	307	317	331	rBV	128462	188843	31.88%	4.036%
4	2.449	431	438	448	rVB	21820	30975	5.23%	0.662%
5	3.902	871	890	891	rBV	30532	58907	9.95%	1.259%
6	4.021	923	927	936	rVB	30331	26891	4.54%	0.575%
7	4.252	985	999	1017	rVB	116336	302915	51.14%	6.473%
8	4.960	1203	1219	1246	rBV3	246074	592307	100.00%	12.658%
9	5.539	1386	1399	1422	rBV2	180934	373816	63.11%	7.988%
10	5.998	1524	1542	1564	rBV2	140211	295894	49.96%	6.323%
11	6.921	1817	1829	1842	rBV2	54355	101068	17.06%	2.160%
12	7.249	1918	1931	1948	rBV	235807	422124	71.27%	9.021%
13	7.561	2019	2028	2050	rBV	31838	57422	9.69%	1.227%
14	7.886	2121	2129	2135	rBV3	7190	10526	1.78%	0.225%
15	8.050	2170	2180	2212	rBV	220697	470744	79.48%	10.060%
16	8.792	2399	2411	2439	rBV	268932	482005	81.38%	10.300%
17	9.082	2492	2501	2510	rVB	13544	22901	3.87%	0.489%
18	9.487	2619	2627	2640	rVB3	9098	14917	2.52%	0.319%
19	9.873	2739	2747	2757	rBV3	7278	11735	1.98%	0.251%
20	10.162	2820	2837	2851	rBV2	97920	159171	26.87%	3.402%
21	10.509	2936	2945	2954	rVB2	9269	16140	2.72%	0.345%
22	11.034	3100	3108	3116	rVB2	7811	11316	1.91%	0.242%
23	11.194	3145	3158	3174	rBV	269098	431194	72.80%	9.215%
24	11.281	3177	3185	3196	rVB2	8988	14806	2.50%	0.316%
25	11.474	3236	3245	3253	rBV	13815	23371	3.95%	0.499%
26	11.567	3263	3274	3289	rBV	252649	399461	67.44%	8.537%
27	12.201	3459	3471	3479	rBV	3235	6157	1.04%	0.132%
28	12.619	3590	3601	3605	rBV	3941	6686	1.13%	0.143%




Sum of corrected areas: 4679434

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030352.D
Acq On : 30 Mar 2023 12:21
Operator : SY/MD
Sample : 02092-19 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB991

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

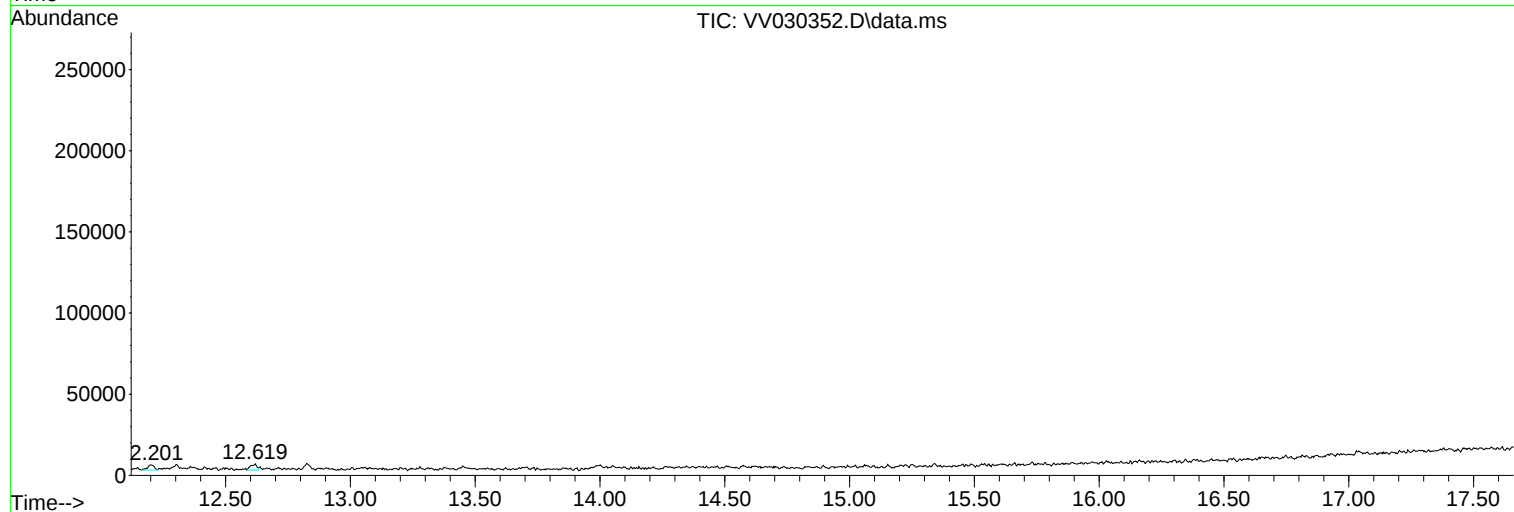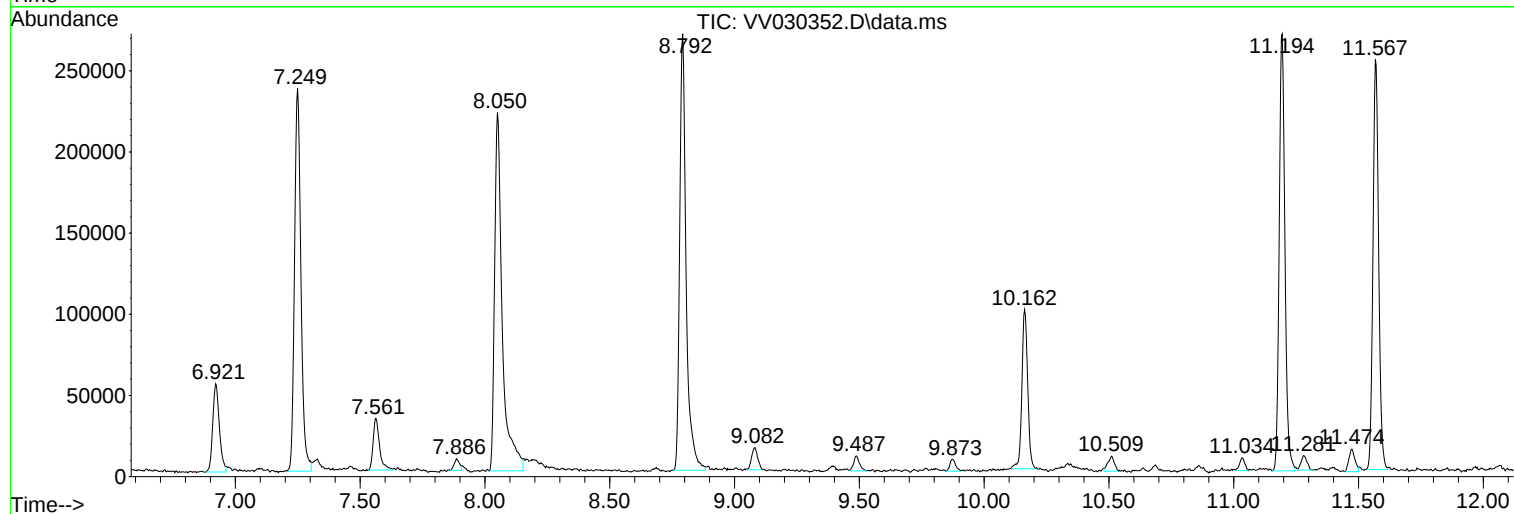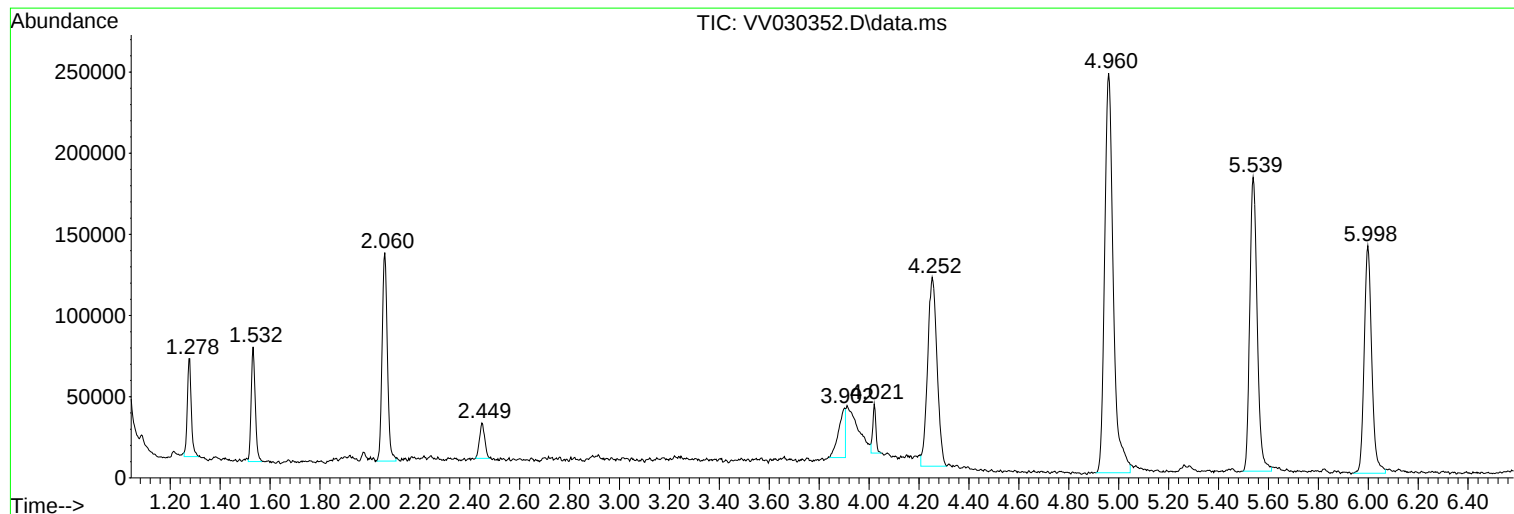

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030352.D
Acq On : 30 Mar 2023 12:21
Operator : SY/MD
Sample : 02092-19 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB991

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030352.D
Acq On : 30 Mar 2023 12:21
Operator : SY/MD
Sample : 02092-19 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB991

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------