

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030353.D
 Acq On : 30 Mar 2023 12:46
 Operator : SY/MD
 Sample : 02092-23 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB998

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	66	75	85	rVB	44475	50790	9.46%	1.206%
2	1.539	147	155	166	rVB	53174	61811	11.52%	1.467%
3	1.982	286	293	302	rBV6	5512	7903	1.47%	0.188%
4	2.063	308	318	331	rBV	97153	144765	26.97%	3.437%
5	2.455	425	440	456	rBV2	19768	35793	6.67%	0.850%
6	3.828	850	867	900	rBV3	43530	186930	34.83%	4.438%
7	4.259	982	1001	1025	rBV2	81125	218061	40.63%	5.177%
8	4.966	1206	1221	1257	rBV3	164949	465970	86.81%	11.062%
9	5.542	1387	1400	1418	rBV	196272	413059	76.95%	9.806%
10	5.998	1527	1542	1559	rBV	103724	220868	41.15%	5.243%
11	6.921	1815	1829	1842	rBV2	41745	82425	15.36%	1.957%
12	7.252	1917	1932	1949	rBV	176497	323124	60.20%	7.671%
13	7.561	2018	2028	2045	rBV	25047	47294	8.81%	1.123%
14	7.879	2120	2127	2134	rBV9	4845	7558	1.41%	0.179%
15	8.037	2163	2176	2210	rBV	178842	400443	74.60%	9.506%
16	8.368	2271	2279	2282	rBV7	5200	6316	1.18%	0.150%
17	8.792	2397	2411	2435	rBV	299976	536756	100.00%	12.742%
18	9.078	2491	2500	2512	rVB5	7190	12521	2.33%	0.297%
19	9.487	2621	2627	2638	rVB6	5258	8635	1.61%	0.205%
20	9.876	2736	2748	2760	rVB6	4796	10168	1.89%	0.241%
21	10.130	2816	2827	2828	rBV9	5851	8490	1.58%	0.202%
22	10.162	2828	2837	2852	rVB	79378	130369	24.29%	3.095%
23	10.512	2938	2946	2954	rVB	6212	10617	1.98%	0.252%
24	11.194	3147	3158	3173	rBV	307991	486797	90.69%	11.556%
25	11.284	3180	3186	3195	rVB8	3962	6209	1.16%	0.147%
26	11.474	3234	3245	3256	rBV9	5901	12144	2.26%	0.288%
27	11.570	3262	3275	3290	rBV	194579	316562	58.98%	7.515%




Sum of corrected areas: 4212378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030353.D
Acq On : 30 Mar 2023 12:46
Operator : SY/MD
Sample : 02092-23 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB998

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

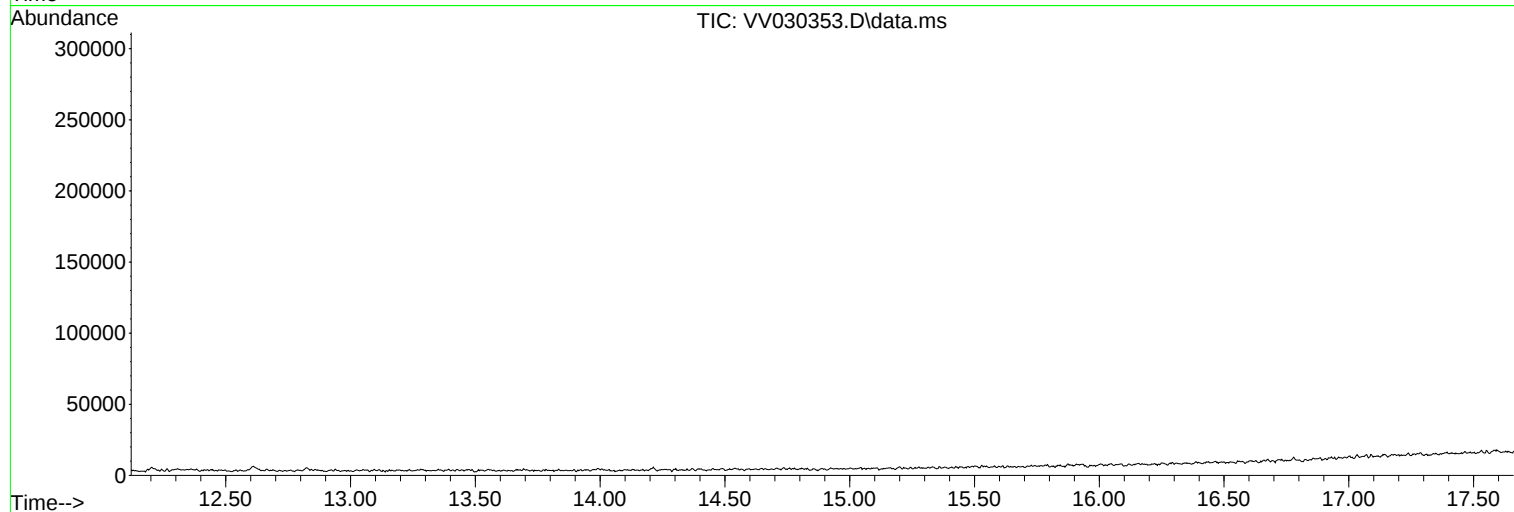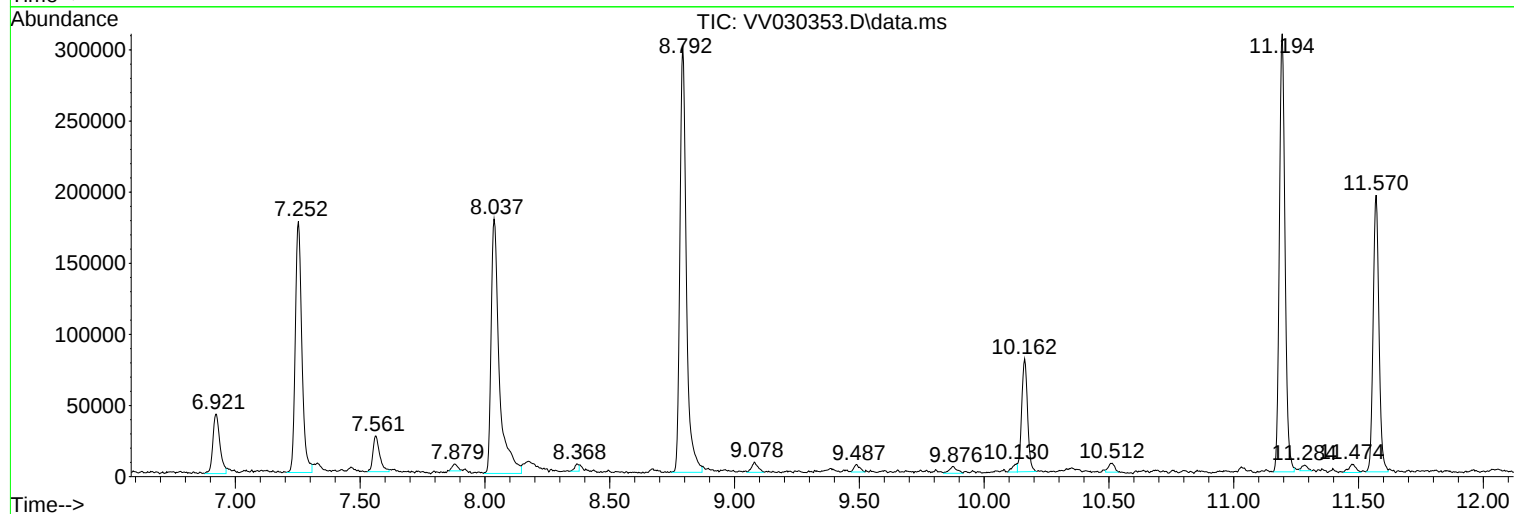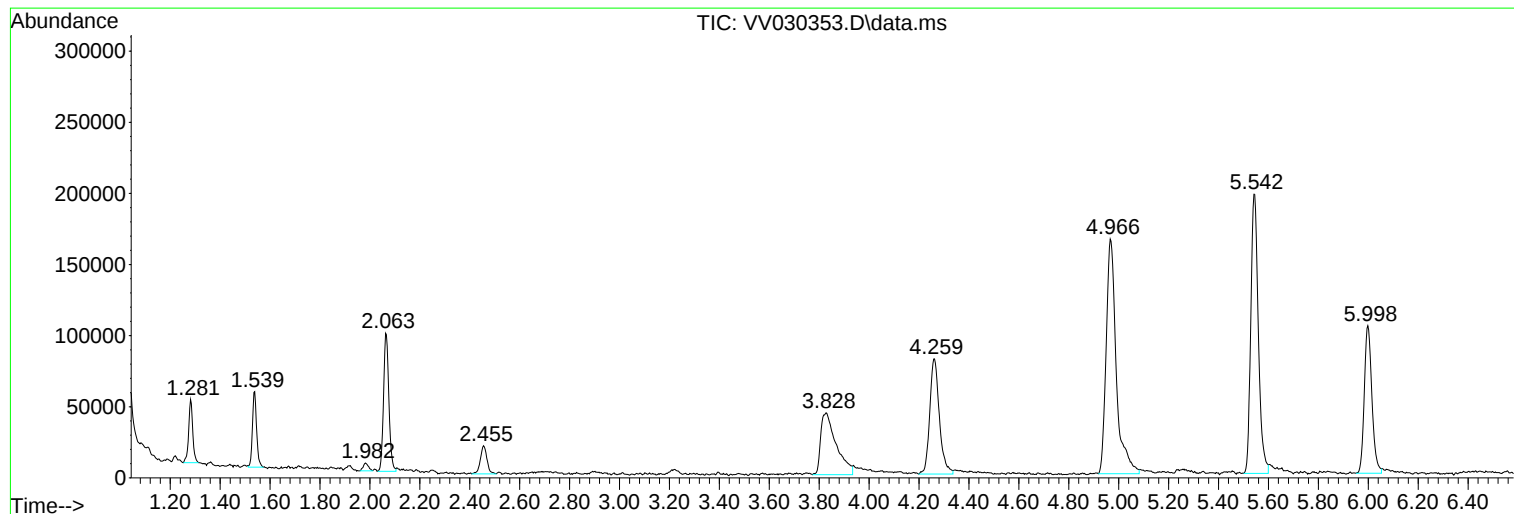

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030353.D
Acq On : 30 Mar 2023 12:46
Operator : SY/MD
Sample : 02092-23 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB998

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030353.D
Acq On : 30 Mar 2023 12:46
Operator : SY/MD
Sample : 02092-23 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB998

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc