

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030354.D
 Acq On : 30 Mar 2023 13:09
 Operator : SY/MD
 Sample : 02122-04 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB9A6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rVB	53466	62404	11.74%	1.385%
2	1.535	147	154	168	rVB	59302	70618	13.29%	1.567%
3	1.986	285	294	304	rBV6	6765	12688	2.39%	0.282%
4	2.066	309	319	333	rVV	104963	158519	29.83%	3.519%
5	2.455	427	440	449	rBV2	19772	34737	6.54%	0.771%
6	3.822	851	865	900	rBV2	51958	212175	39.93%	4.710%
7	4.262	984	1002	1021	rBV	90816	238482	44.88%	5.293%
8	4.969	1203	1222	1253	rBV3	187195	531370	100.00%	11.794%
9	5.542	1385	1400	1420	rBV	197912	422713	79.55%	9.383%
10	5.998	1528	1542	1566	rBV	117635	251191	47.27%	5.576%
11	6.921	1814	1829	1843	rBV2	48282	95719	18.01%	2.125%
12	7.252	1919	1932	1954	rBV	203960	375500	70.67%	8.335%
13	7.561	2017	2028	2042	rBV3	29217	57226	10.77%	1.270%
14	8.037	2166	2176	2206	rBV	219703	456554	85.92%	10.134%
15	8.792	2399	2411	2433	rBV	306571	529252	99.60%	11.747%
16	10.162	2826	2837	2852	rVB	87906	143642	27.03%	3.188%
17	11.033	3099	3108	3114	rBV	5984	8964	1.69%	0.199%
18	11.194	3146	3158	3174	rBV	311498	490138	92.24%	10.879%
19	11.570	3259	3275	3288	rBV	218426	353344	66.50%	7.843%




Sum of corrected areas: 4505236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030354.D
Acq On : 30 Mar 2023 13:09
Operator : SY/MD
Sample : 02122-04 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

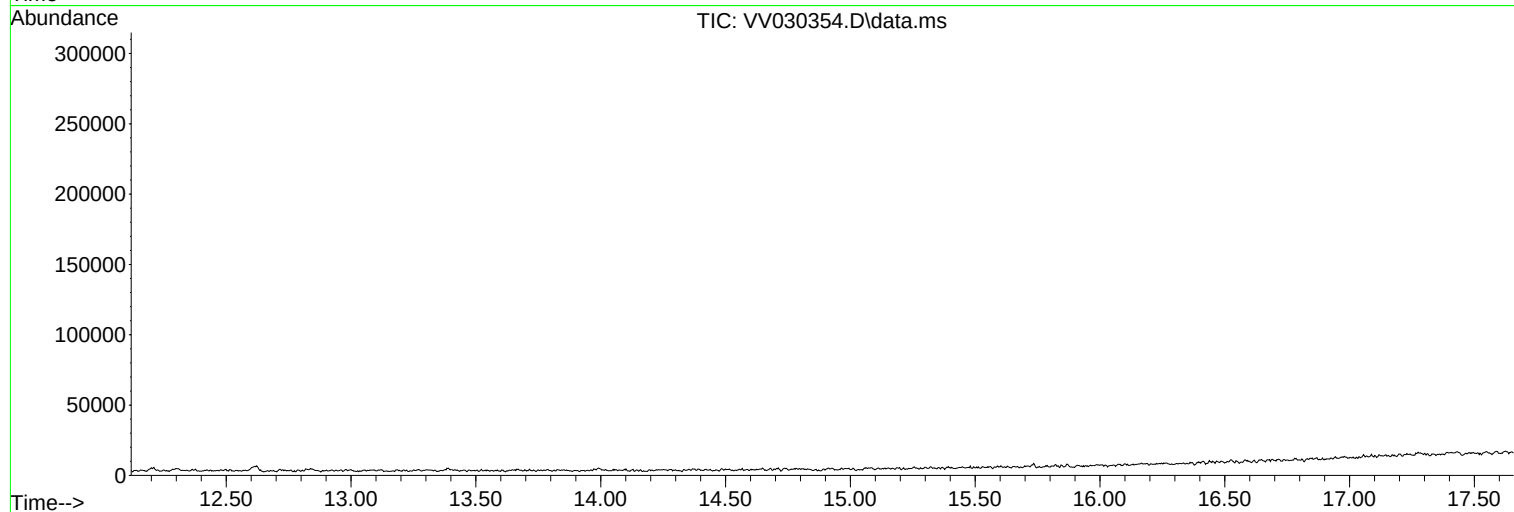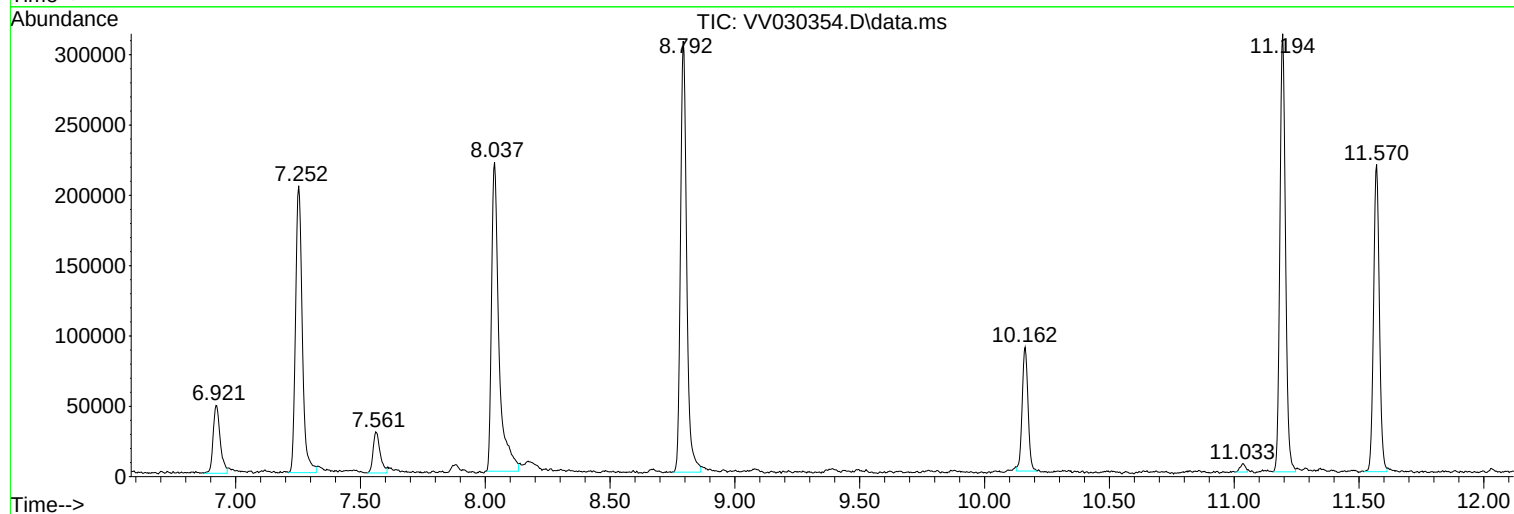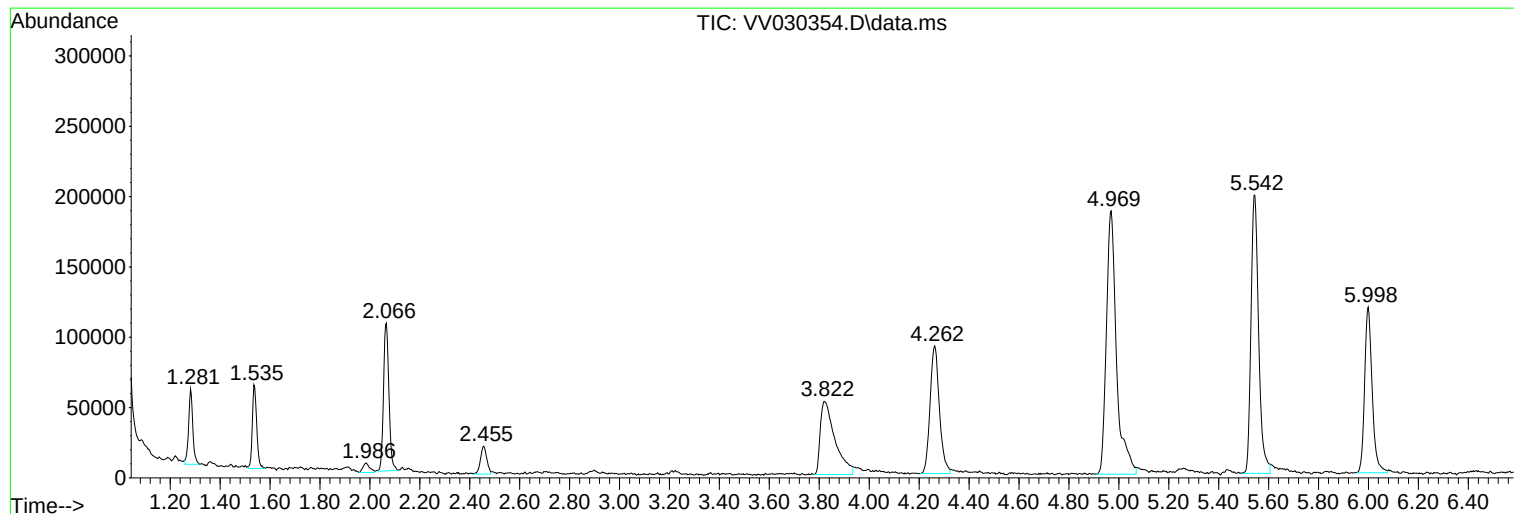

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030354.D
Acq On : 30 Mar 2023 13:09
Operator : SY/MD
Sample : 02122-04 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030354.D
Acq On : 30 Mar 2023 13:09
Operator : SY/MD
Sample : 02122-04 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------