

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030355.D
 Acq On : 30 Mar 2023 13:34
 Operator : SY/MD
 Sample : 02122-02 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB9A2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	83	rBV	57130	62589	10.39%	1.257%
2	1.539	148	155	165	rVB	64920	74442	12.36%	1.495%
3	1.986	284	294	302	rBV3	7704	12692	2.11%	0.255%
4	2.066	307	319	332	rBV	117119	174926	29.05%	3.514%
5	2.452	425	439	453	rBV	20189	37601	6.24%	0.755%
6	3.822	852	865	906	rBV2	49046	194666	32.33%	3.911%
7	4.259	983	1001	1020	rBV	98922	256734	42.63%	5.158%
8	4.969	1202	1222	1258	rBV3	203830	602172	100.00%	12.097%
9	5.542	1385	1400	1417	rBV	205870	427637	71.02%	8.591%
10	5.998	1525	1542	1558	rBV2	128316	271500	45.09%	5.454%
11	6.921	1818	1829	1845	rBV	53025	101703	16.89%	2.043%
12	7.252	1918	1932	1950	rBV	226728	409501	68.00%	8.226%
13	7.561	2013	2028	2041	rBV	31643	61547	10.22%	1.236%
14	7.876	2118	2126	2132	rBV7	5815	9175	1.52%	0.184%
15	8.037	2163	2176	2209	rBV	222869	471493	78.30%	9.472%
16	8.792	2399	2411	2438	rBV	319819	579890	96.30%	11.649%
17	9.082	2491	2501	2514	rBV2	17628	30640	5.09%	0.616%
18	9.490	2617	2628	2641	rVB3	10398	20494	3.40%	0.412%
19	9.876	2736	2748	2762	rBV3	9987	17930	2.98%	0.360%
20	10.162	2826	2837	2853	rVB	95871	156679	26.02%	3.148%
21	10.487	2931	2938	2948	rVB	3722	6499	1.08%	0.131%
22	10.683	2993	2999	3008	rVB3	5686	6914	1.15%	0.139%
23	11.033	3100	3108	3119	rVB3	9872	15668	2.60%	0.315%
24	11.194	3145	3158	3175	rBV	318748	510649	84.80%	10.258%
25	11.281	3177	3185	3194	rVB	15426	23701	3.94%	0.476%
26	11.474	3233	3245	3259	rBV2	16924	28600	4.75%	0.575%
27	11.570	3262	3275	3293	rBV	244725	402822	66.89%	8.092%
28	12.831	3660	3667	3676	rVB10	5254	8990	1.49%	0.181%




Sum of corrected areas: 4977854

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030355.D
Acq On : 30 Mar 2023 13:34
Operator : SY/MD
Sample : 02122-02 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

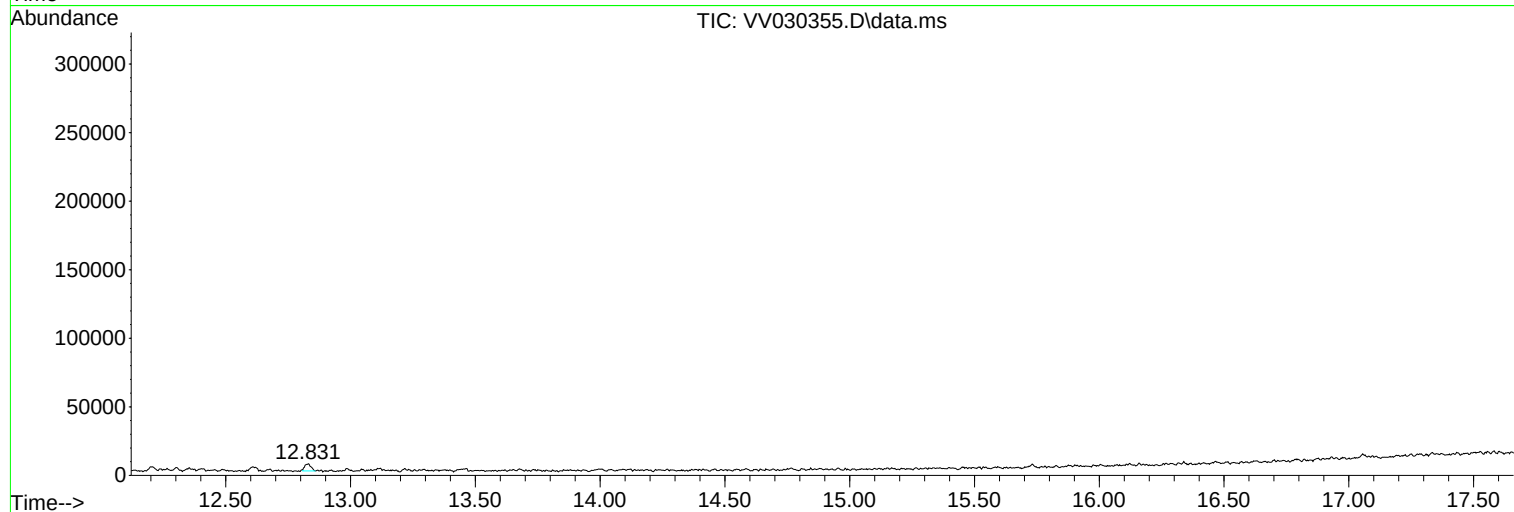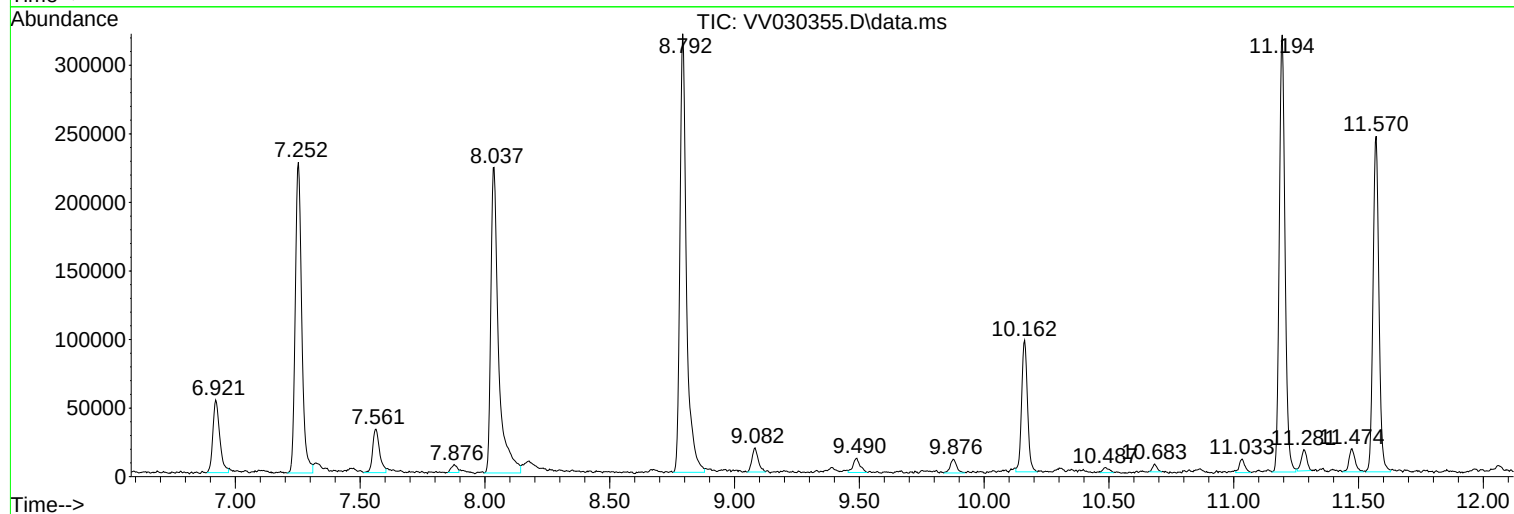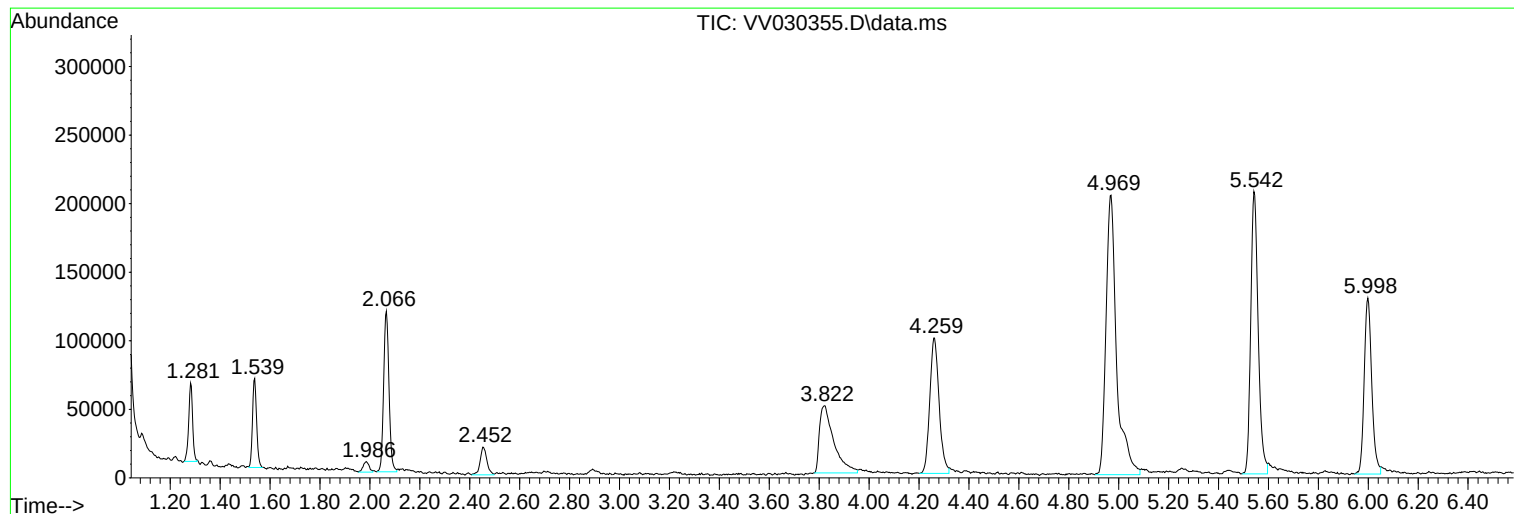

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030355.D
Acq On : 30 Mar 2023 13:34
Operator : SY/MD
Sample : 02122-02 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030355.D
Acq On : 30 Mar 2023 13:34
Operator : SY/MD
Sample : 02122-02 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------