

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030357.D
 Acq On : 30 Mar 2023 14:20
 Operator : SY/MD
 Sample : 02132-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	87	rVB	52174	58729	11.88%	1.381%
2	1.539	147	155	164	rBV	57234	68429	13.84%	1.609%
3	2.066	309	319	335	rBV	106333	156213	31.60%	3.673%
4	3.815	852	863	894	rBV2	54264	191072	38.65%	4.492%
5	4.262	983	1002	1028	rBV	93254	241878	48.92%	5.687%
6	4.969	1206	1222	1245	rBV2	191899	494387	100.00%	11.624%
7	5.545	1389	1401	1421	rBV	167228	351557	71.11%	8.265%
8	5.847	1482	1495	1496	rBV	9367	12537	2.54%	0.295%
9	5.998	1526	1542	1560	rBV	121520	262817	53.16%	6.179%
10	6.924	1819	1830	1851	rBV2	49234	98901	20.00%	2.325%
11	7.252	1920	1932	1947	rBV	206947	371982	75.24%	8.746%
12	7.326	1948	1955	1971	rVB	27667	55139	11.15%	1.296%
13	7.561	2018	2028	2051	rBV	30337	60702	12.28%	1.427%
14	8.037	2163	2176	2205	rBV	221427	464386	93.93%	10.918%
15	8.792	2397	2411	2438	rBV	257726	447975	90.61%	10.532%
16	10.162	2824	2837	2855	rBV	90714	149610	30.26%	3.517%
17	10.339	2882	2892	2898	rVB10	3293	6182	1.25%	0.145%
18	11.194	3141	3158	3179	rVB	251397	399089	80.72%	9.383%
19	11.513	3247	3257	3263	rBV10	4595	9801	1.98%	0.230%
20	11.570	3263	3275	3292	rVB	218329	351925	71.18%	8.274%




Sum of corrected areas: 4253311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030357.D
Acq On : 30 Mar 2023 14:20
Operator : SY/MD
Sample : 02132-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

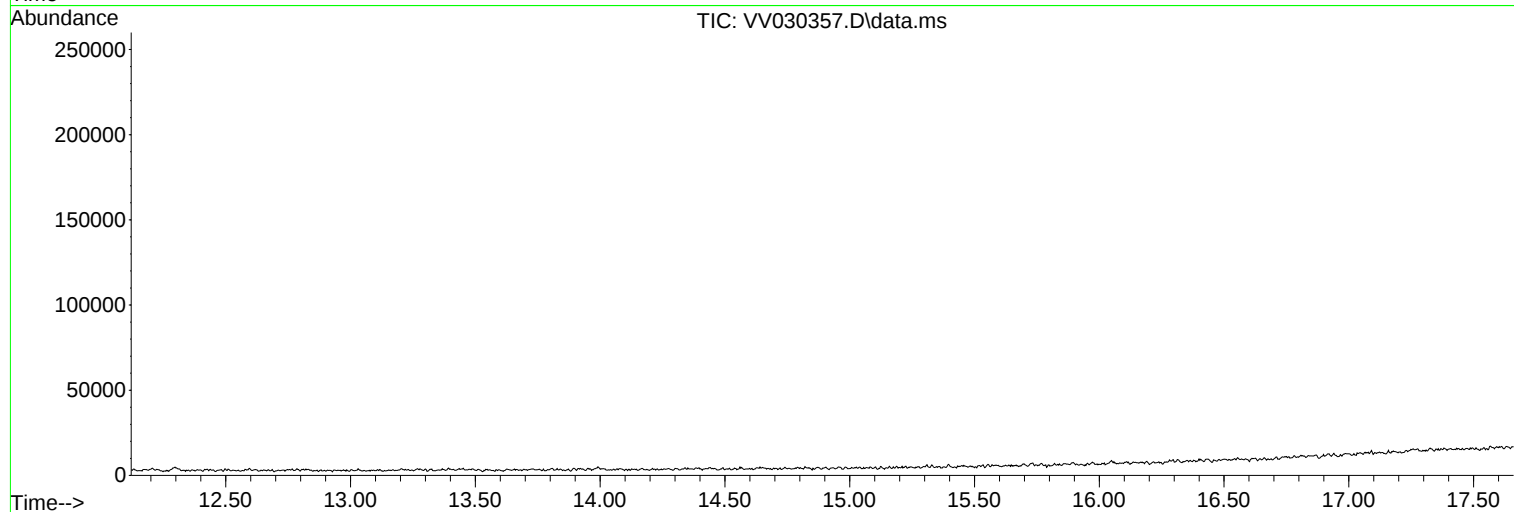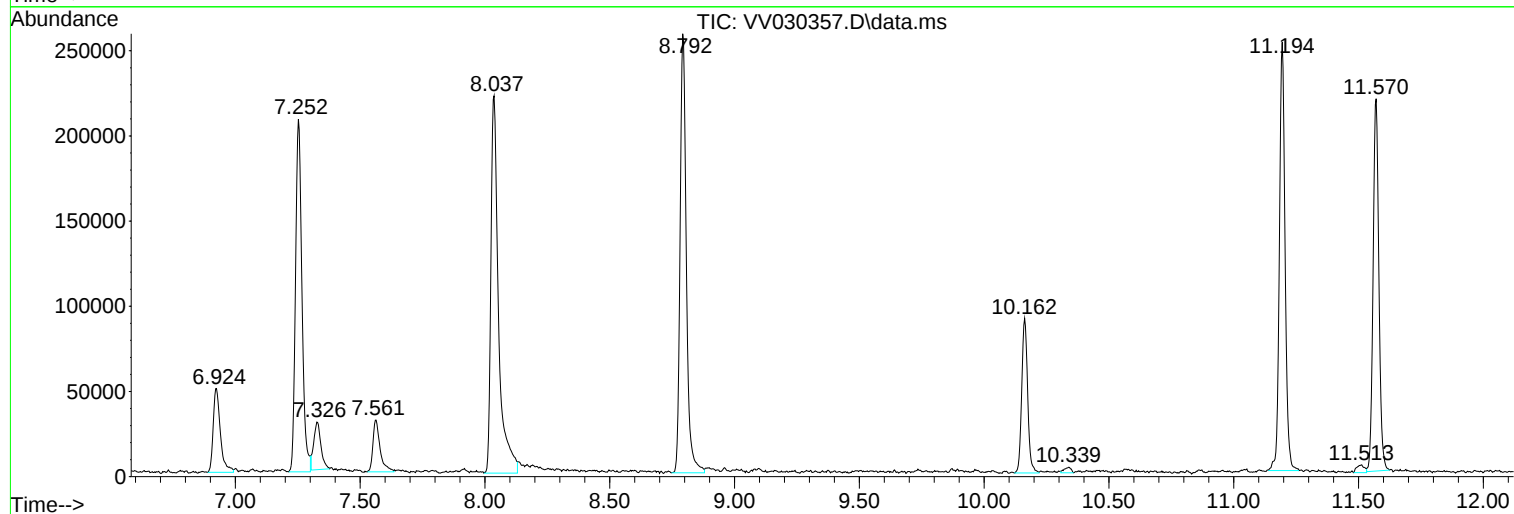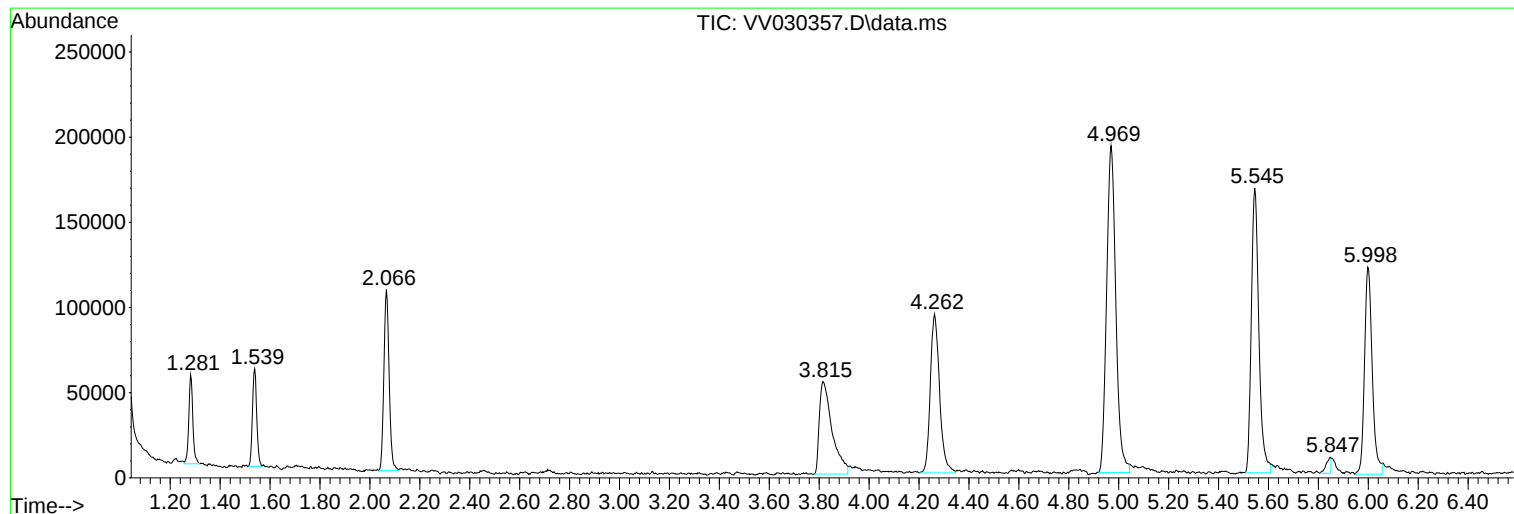

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030357.D
Acq On : 30 Mar 2023 14:20
Operator : SY/MD
Sample : 02132-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030357.D
Acq On : 30 Mar 2023 14:20
Operator : SY/MD
Sample : 02132-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc