

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030360.D
 Acq On : 30 Mar 2023 15:34
 Operator : SY/MD
 Sample : 02132-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	49	57	61	rBV6	4537	8184	1.63%	0.192%
2	1.275	64	73	88	rVB2	58622	80961	16.14%	1.895%
3	1.532	146	153	164	rVB	62638	70908	14.14%	1.659%
4	2.060	307	317	328	rBV	113669	162022	32.30%	3.792%
5	3.751	839	843	851	rVB	9499	10714	2.14%	0.251%
6	3.905	869	891	916	rBV2	34123	175059	34.90%	4.097%
7	4.252	983	999	1018	rBV	95785	238876	47.62%	5.590%
8	4.960	1201	1219	1241	rBV3	213025	501631	100.00%	11.739%
9	5.539	1384	1399	1418	rBV	150552	316672	63.13%	7.411%
10	5.998	1526	1542	1557	rBV2	121222	256976	51.23%	6.014%
11	6.921	1818	1829	1844	rBV2	45863	87588	17.46%	2.050%
12	7.249	1915	1931	1947	rBV	206746	366140	72.99%	8.568%
13	7.323	1951	1954	1963	rVB4	8078	12409	2.47%	0.290%
14	7.564	2014	2029	2045	rBV	29152	58198	11.60%	1.362%
15	8.050	2169	2180	2200	rBV	212121	444142	88.54%	10.394%
16	8.792	2399	2411	2428	rBV	222926	376412	75.04%	8.809%
17	10.162	2826	2837	2855	rVB	91377	150295	29.96%	3.517%
18	10.336	2883	2891	2901	rVB	7546	11546	2.30%	0.270%
19	11.194	3144	3158	3178	rBV	214960	346356	69.05%	8.105%
20	11.493	3241	3251	3264	rBV	89662	191752	38.23%	4.487%
21	11.567	3265	3274	3292	rVB	244339	398099	79.36%	9.316%
22	12.204	3463	3472	3480	rBV8	5094	8173	1.63%	0.191%




Sum of corrected areas: 4273113

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030360.D
Acq On : 30 Mar 2023 15:34
Operator : SY/MD
Sample : 02132-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

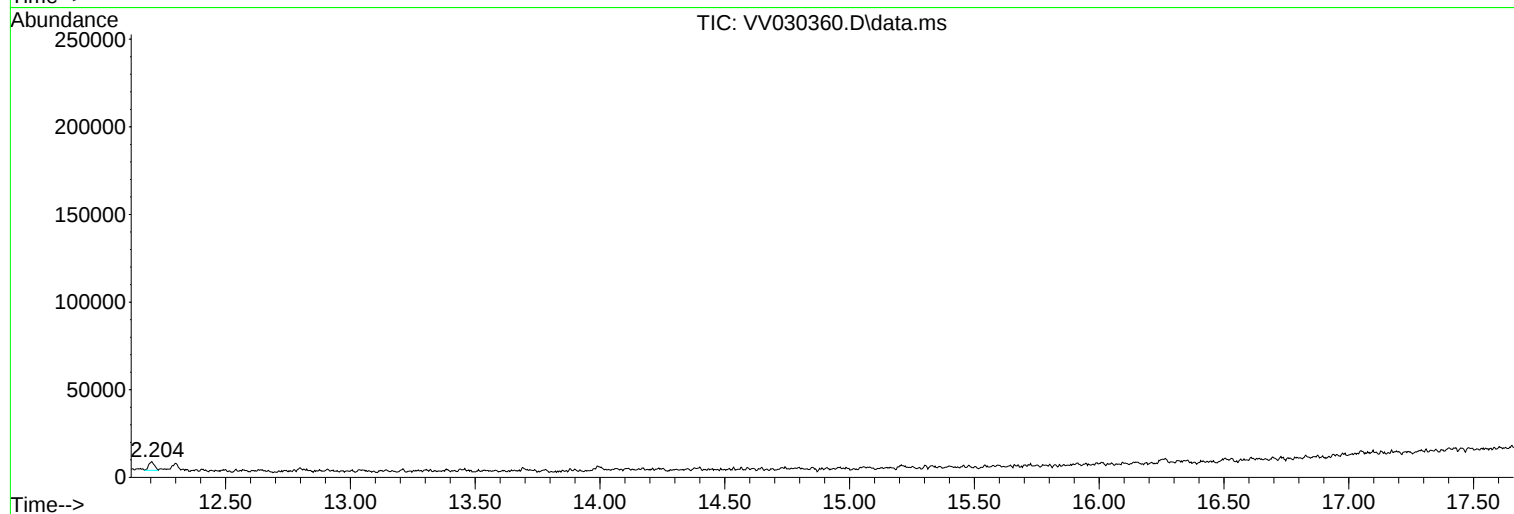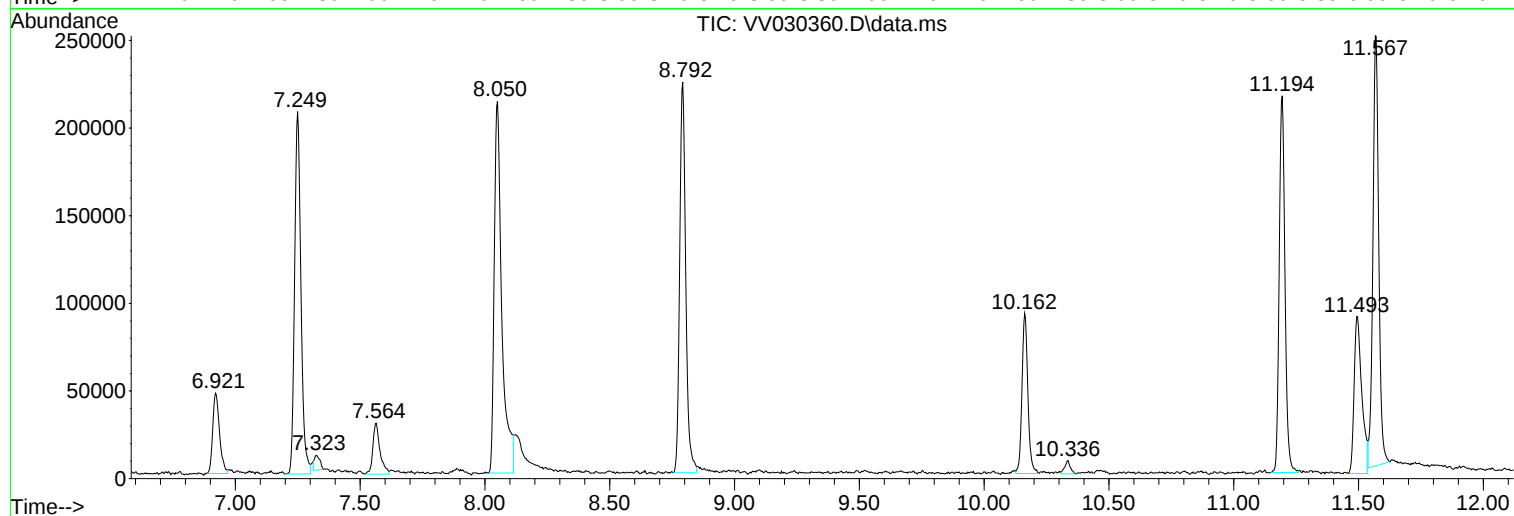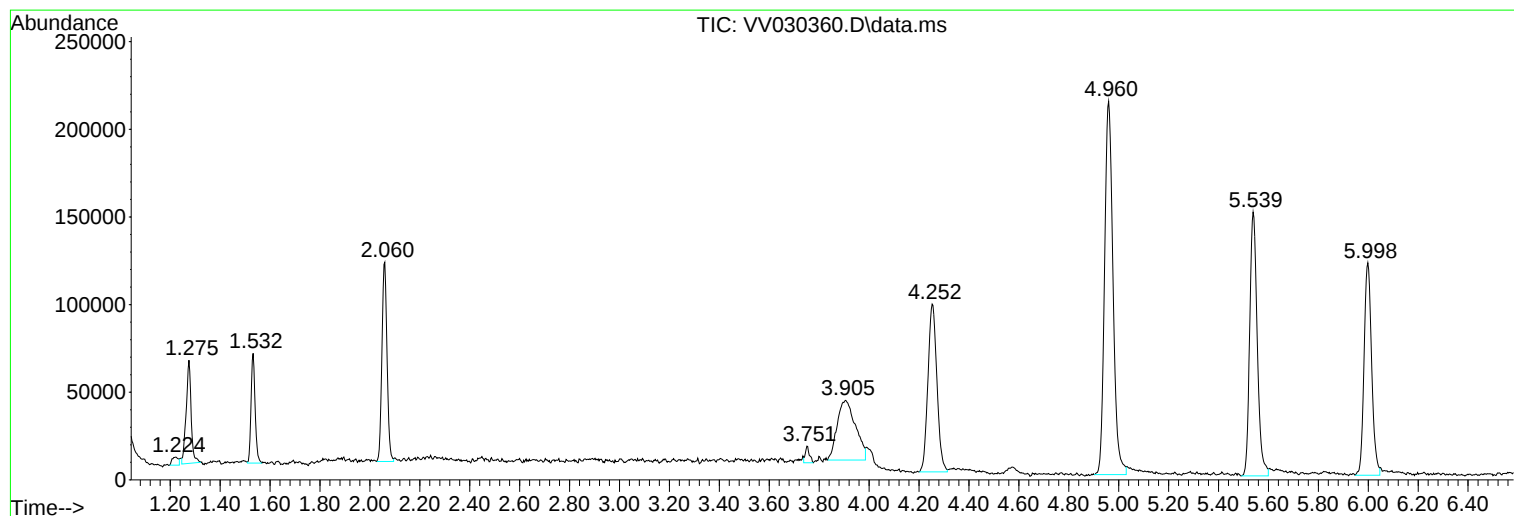

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030360.D
Acq On : 30 Mar 2023 15:34
Operator : SY/MD
Sample : 02132-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMB7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.493	2.77 ug/L	191752	1,4-Dichlorobenzene-d4	11.194

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
5	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	59

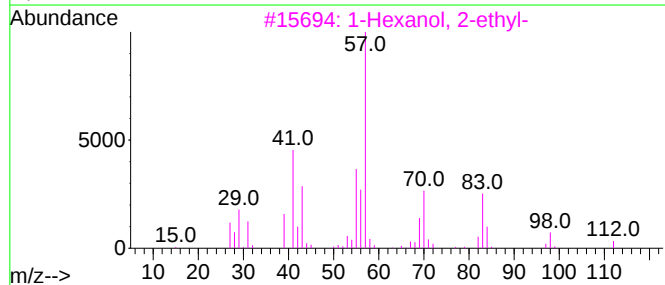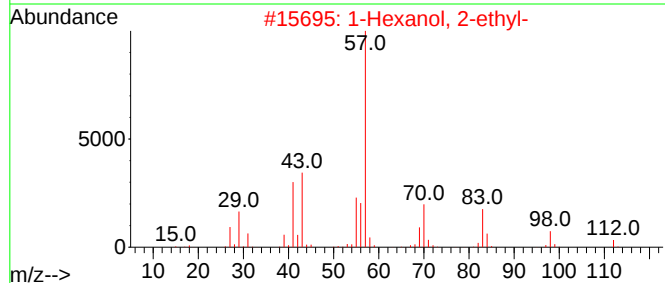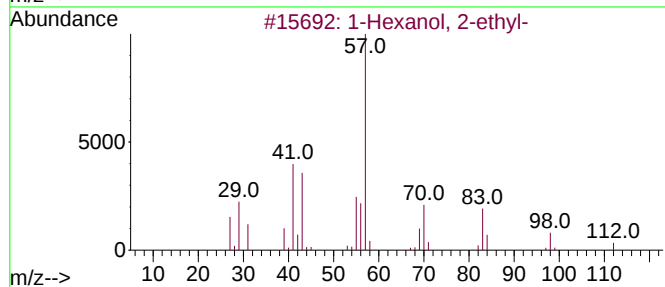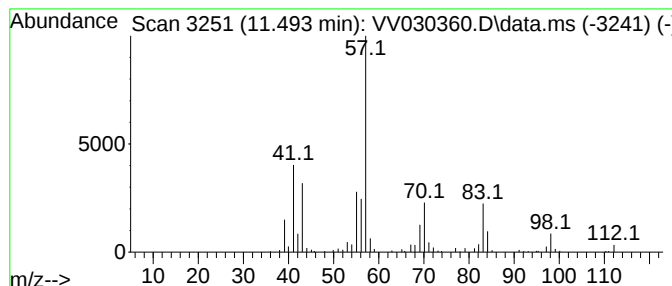

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030360.D
Acq On : 30 Mar 2023 15:34
Operator : SY/MD
Sample : 02132-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.493	2.8	ug/L	191752	3	11.194	346356	5.0