

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030366.D
 Acq On : 30 Mar 2023 17:54
 Operator : SY/MD
 Sample : 02130-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11B7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	60	rBV2	6563	7587	1.32%	0.162%
2	1.278	66	74	90	rVB	54287	61736	10.70%	1.322%
3	1.536	147	154	168	rVB	65346	78080	13.54%	1.672%
4	2.063	306	318	330	rBV	118070	175365	30.40%	3.756%
5	3.841	859	871	911	rBV	33377	193524	33.55%	4.145%
6	4.262	983	1002	1026	rBV2	98698	267100	46.31%	5.721%
7	4.970	1199	1222	1250	rBV2	219892	576791	100.00%	12.354%
8	5.545	1381	1401	1424	rBV	162043	349656	60.62%	7.489%
9	5.998	1530	1542	1559	rBV2	132294	274512	47.59%	5.880%
10	6.921	1819	1829	1852	rBV	53459	106611	18.48%	2.283%
11	7.252	1919	1932	1956	rBV	236957	435907	75.57%	9.336%
12	7.564	2019	2029	2044	rBV2	32551	62962	10.92%	1.349%
13	8.037	2164	2176	2214	rBV	250022	561092	97.28%	12.018%
14	8.793	2399	2411	2436	rBV	244861	418746	72.60%	8.969%
15	10.162	2825	2837	2855	rVB	100887	166049	28.79%	3.556%
16	11.104	3121	3130	3135	rBV9	5749	8257	1.43%	0.177%
17	11.194	3146	3158	3175	rBV	255434	398181	69.03%	8.528%
18	11.497	3237	3252	3264	rBV2	28022	64304	11.15%	1.377%
19	11.571	3264	3275	3290	rVB	259338	415346	72.01%	8.896%
20	12.297	3492	3501	3513	rVB3	23302	34761	6.03%	0.745%
21	16.429	4782	4786	4796	rVB7	7876	12373	2.15%	0.265%




Sum of corrected areas: 4668940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030366.D
Acq On : 30 Mar 2023 17:54
Operator : SY/MD
Sample : 02130-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

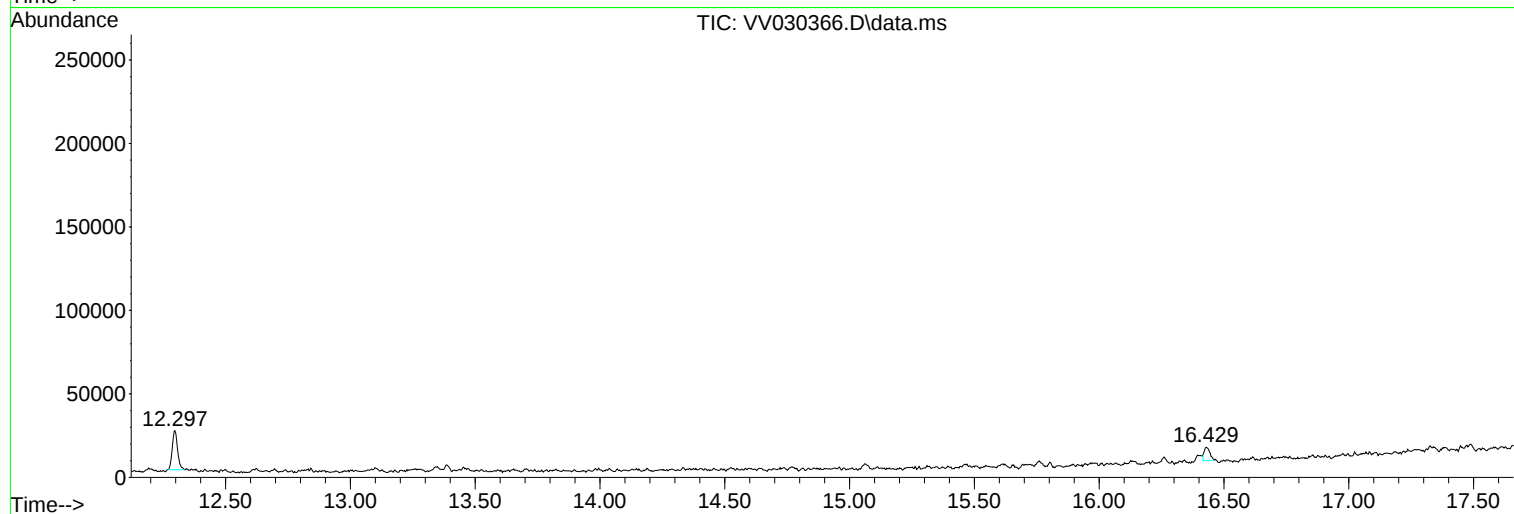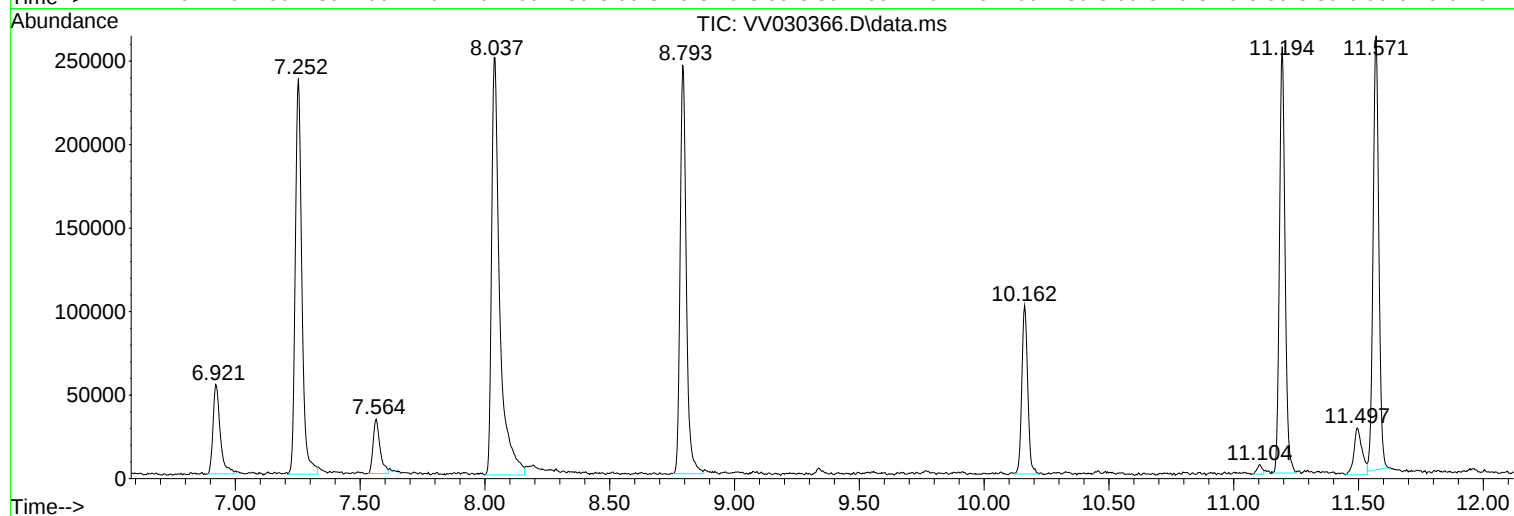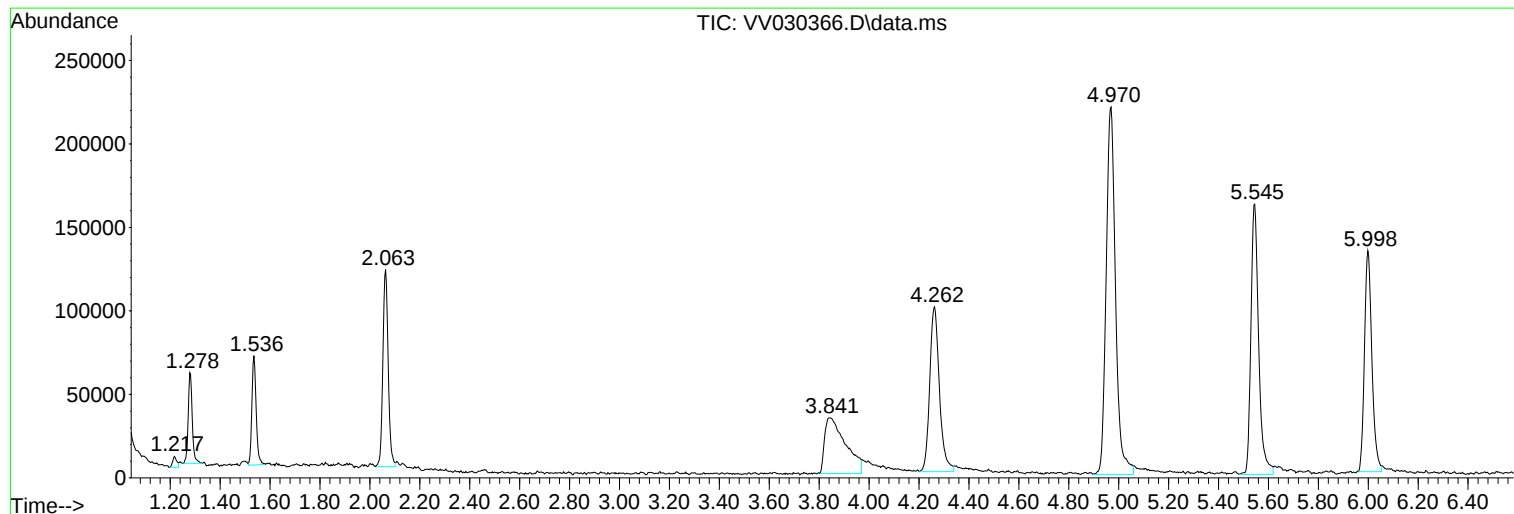

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030366.D
Acq On : 30 Mar 2023 17:54
Operator : SY/MD
Sample : 02130-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11B7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.497	0.81 ug/L	64304	1,4-Dichlorobenzene-d4	11.194

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	90
2		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	90
3		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	83
4		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	83
5		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	78

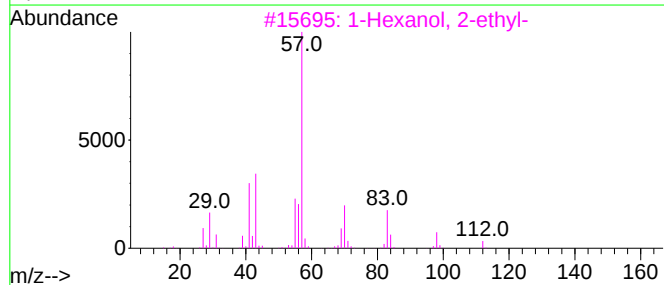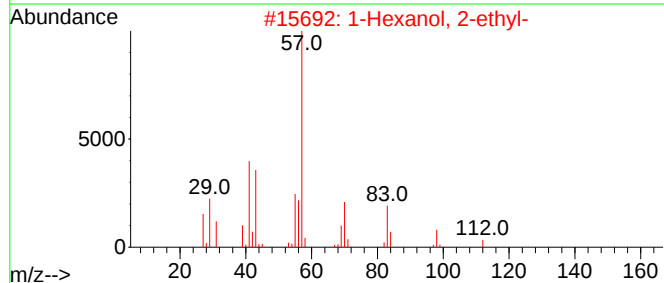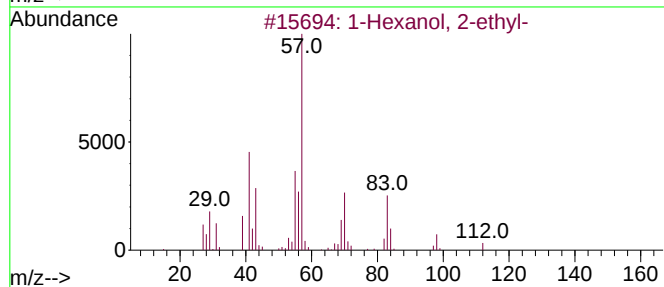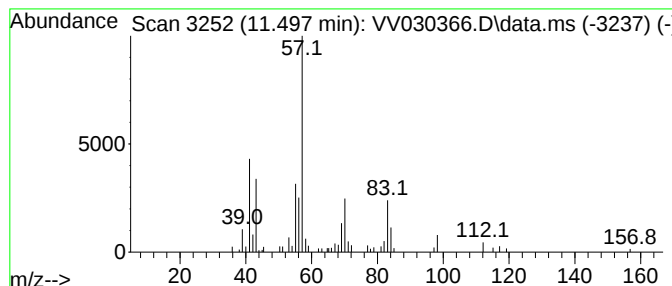

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030366.D
Acq On : 30 Mar 2023 17:54
Operator : SY/MD
Sample : 02130-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.497	0.8	ug/L	64304	3	11.194	398181	5.0