

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
 Data File : VV030368.D
 Acq On : 30 Mar 2023 18:43
 Operator : SY/MD
 Sample : 02130-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rVB	57122	59820	11.16%	1.370%
2	1.536	146	154	168	rBV	63748	74311	13.86%	1.702%
3	2.066	309	319	331	rBV	114322	168271	31.39%	3.854%
4	2.455	428	440	448	rBV	8022	13726	2.56%	0.314%
5	3.815	851	863	899	rBV2	56666	212661	39.67%	4.871%
6	4.262	982	1002	1021	rBV	95974	245757	45.84%	5.629%
7	4.966	1205	1221	1245	rBV3	205516	536072	100.00%	12.279%
8	5.542	1389	1400	1422	rBV	161475	336778	62.82%	7.714%
9	5.998	1527	1542	1558	rBV2	124605	265929	49.61%	6.091%
10	6.921	1817	1829	1848	rBV	50942	102171	19.06%	2.340%
11	7.252	1920	1932	1951	rBV	225215	407743	76.06%	9.340%
12	7.561	2018	2028	2044	rBV	30928	60837	11.35%	1.393%
13	8.034	2166	2175	2210	rBV	245695	500943	93.45%	11.474%
14	8.375	2271	2281	2289	rBV3	7708	13650	2.55%	0.313%
15	8.793	2399	2411	2432	rBV	247234	422884	78.89%	9.686%
16	10.162	2825	2837	2849	rBV	90959	152072	28.37%	3.483%
17	11.194	3146	3158	3175	rBV	251022	398361	74.31%	9.125%
18	11.571	3263	3275	3290	rBV	235077	373238	69.62%	8.549%
19	12.297	3491	3501	3512	rBV	4384	7348	1.37%	0.168%
20	17.049	4973	4979	4993	rVB3	6760	13216	2.47%	0.303%




Sum of corrected areas: 4365788

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030368.D
Acq On : 30 Mar 2023 18:43
Operator : SY/MD
Sample : 02130-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

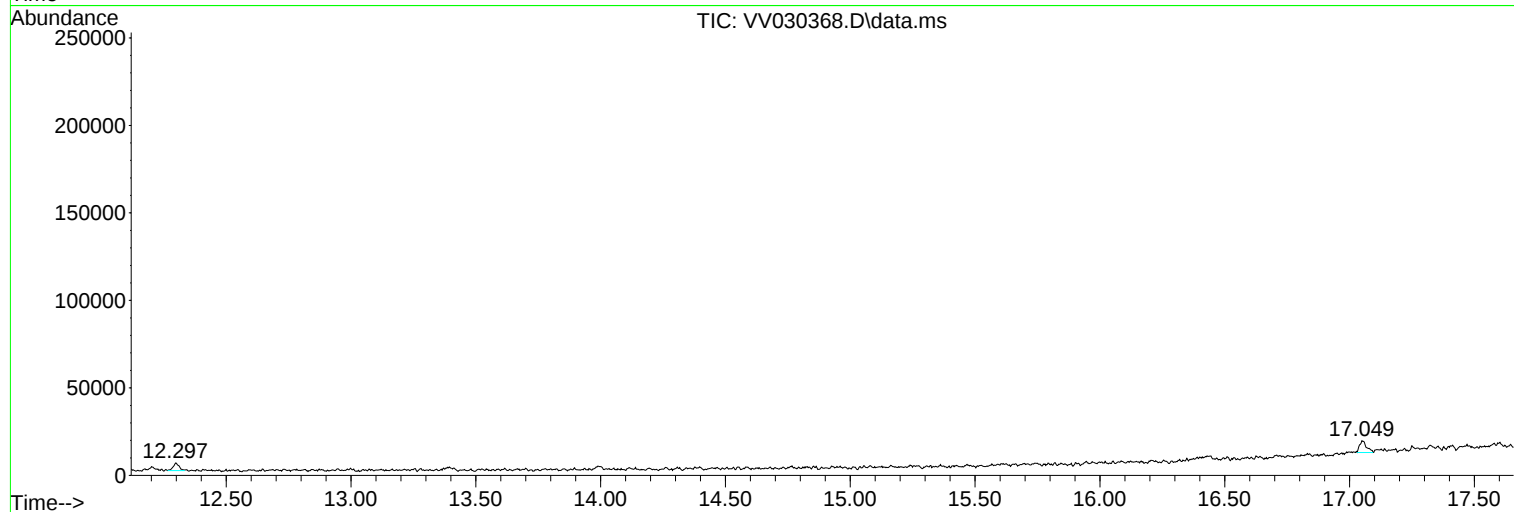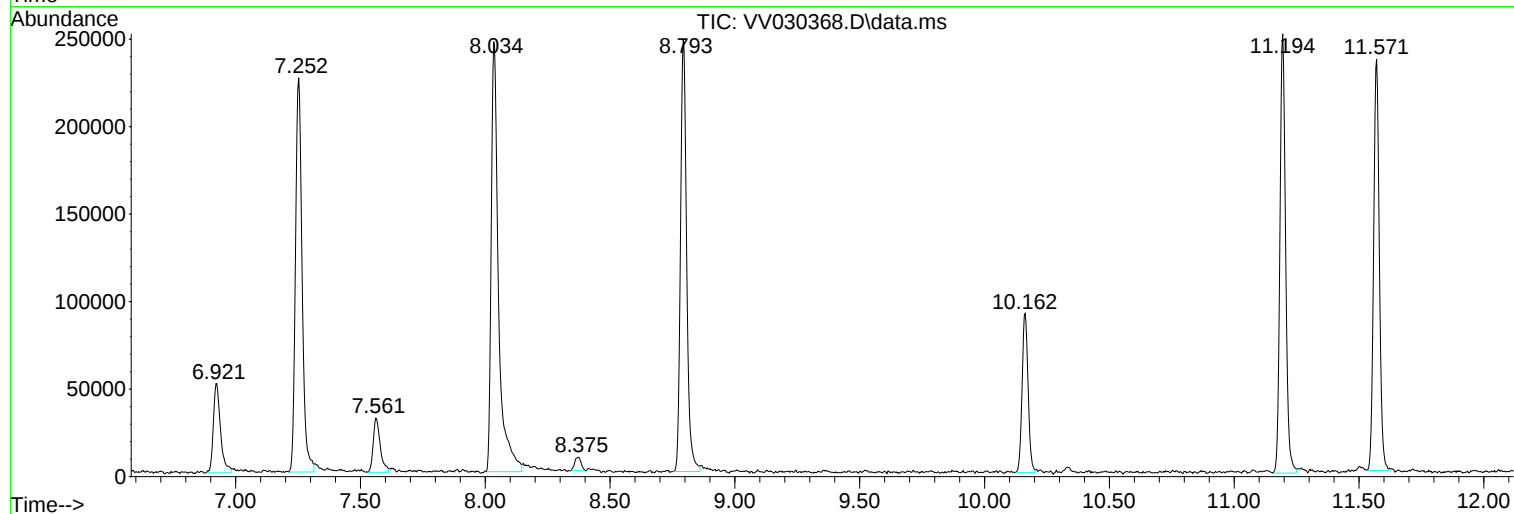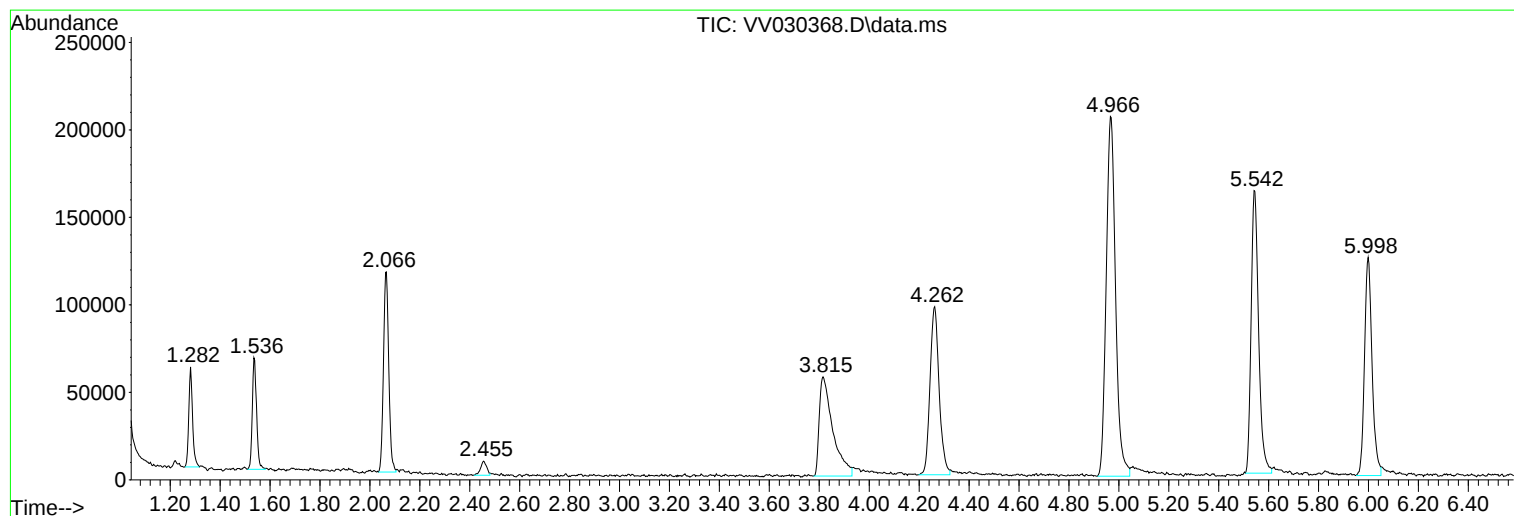

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030368.D
Acq On : 30 Mar 2023 18:43
Operator : SY/MD
Sample : 02130-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030368.D
Acq On : 30 Mar 2023 18:43
Operator : SY/MD
Sample : 02130-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc