
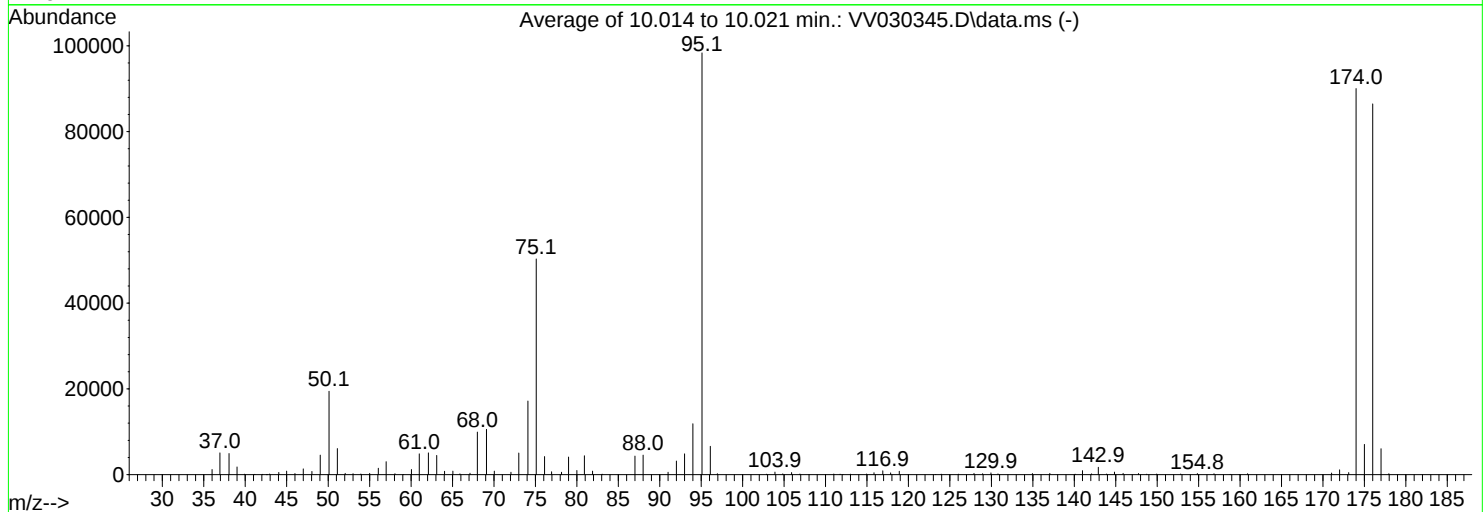


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033023\
Data File : VV030345.D
Acq On : 30 Mar 2023 08:54
Operator : SY/MD
Sample : BFB240
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB240

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 31 05:37:21 2023

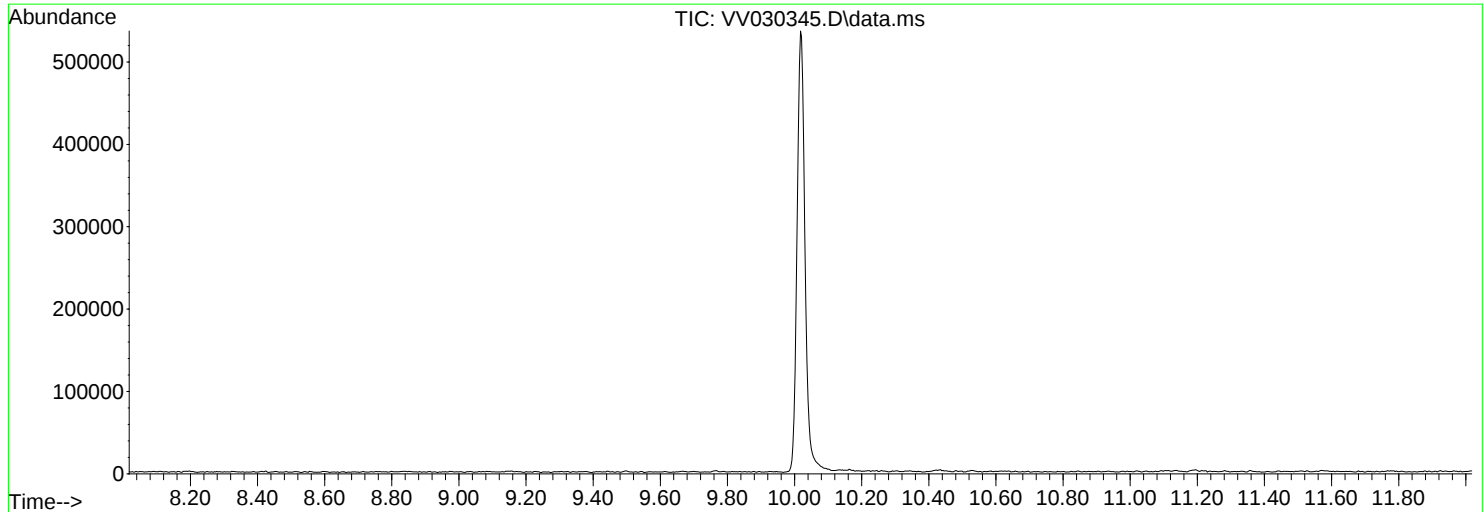

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	19440	PASS
75	95	30	80	51.1	50296	PASS
95	95	100	100	100.0	98373	PASS
96	95	5	9	6.7	6595	PASS
173	174	0.00	2	0.5	478	PASS
174	95	50	120	91.5	90053	PASS
175	174	5	9	7.8	7036	PASS
176	174	95	105	96.0	86483	PASS
177	176	5	10	7.0	6033	PASS

m/z	Abundance
35.10	165.0
36.20	104.0
36.90	133.0
37.30	103.0
38.00	136.0
39.00	143.0
39.90	190.0
41.40	142.0
42.70	118.0
44.00	326.0
45.10	115.0
45.60	140.0
49.50	103.0
54.30	125.0
55.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.30	176.0
36.00	1304.0
37.00	5035.0
38.10	4899.0
39.00	1871.0
39.90	307.0
41.10	151.0
42.10	119.0
42.90	156.0
44.10	868.0
45.00	849.0
46.00	261.0
47.00	1275.0
48.00	709.0
49.10	4314.0
50.10	18768.0
51.10	5919.0
52.20	288.0
53.00	218.0
54.00	132.0
55.00	388.0
56.00	1601.0
57.00	3083.0
58.10	217.0
59.10	106.0
60.10	1143.0
61.00	4603.0
62.10	4917.0
63.10	4379.0
64.00	716.0
65.10	751.0
65.90	185.0
67.10	286.0
68.00	9422.0
69.10	10236.0
70.00	742.0
72.10	534.0
73.00	4918.0
74.10	16808.0
75.10	48112.0
76.10	4220.0
77.00	625.0
78.20	544.0
79.00	3948.0
80.00	910.0
80.90	4257.0
81.90	736.0
83.00	106.0
87.00	4129.0
88.00	4604.0
91.00	593.0
92.00	3107.0
93.00	4577.0
94.00	11544.0
95.10	94632.0
96.10	6384.0
97.00	240.0
103.00	110.0
103.90	506.0
104.80	213.0
105.90	443.0
106.90	149.0
111.00	141.0
111.70	127.0
113.00	104.0
114.90	157.0
115.80	445.0
116.90	806.0
117.80	446.0
118.90	645.0
123.30	107.0
123.90	116.0
126.00	102.0
127.90	290.0
129.00	243.0
129.90	329.0
130.80	192.0
135.00	222.0
137.10	282.0
140.10	135.0
141.00	912.0
142.10	204.0
142.90	1684.0
143.90	131.0
144.80	586.0
145.90	274.0
147.70	225.0
148.70	107.0
150.10	140.0
152.80	147.0
154.90	266.0
156.90	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

160.90	224.0
171.10	316.0
172.00	1038.0
173.10	1435.0
174.00	83648.0
175.00	6555.0
176.00	79872.0
177.00	5502.0
177.90	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.30	161.0
36.00	1344.0
37.00	5382.0
38.10	5273.0
39.00	1981.0
39.90	318.0
41.20	126.0
42.10	138.0
42.50	180.0
43.00	155.0
44.10	867.0
45.00	986.0
46.00	287.0
47.00	1371.0
48.10	783.0
49.00	4711.0
50.10	20016.0
51.10	6299.0
52.00	313.0
53.00	258.0
53.90	151.0
55.00	438.0
56.10	1502.0
57.00	3133.0
58.10	216.0
60.10	1236.0
61.00	4983.0
62.10	5237.0
63.10	4616.0
64.10	801.0
65.10	820.0
65.90	191.0
67.10	330.0
68.00	10240.0
69.10	10956.0
70.10	830.0
72.00	574.0
73.00	5260.0
74.10	17648.0
75.10	51632.0
76.10	4363.0
76.90	719.0
78.10	578.0
79.00	4240.0
80.00	968.0
80.90	4541.0
81.90	838.0
83.00	134.0
87.00	4480.0
88.00	4751.0
91.00	596.0
92.00	3304.0
93.00	5053.0
94.00	12185.0
95.10	101616.0
96.10	6747.0
96.90	234.0
102.90	136.0
103.90	610.0
104.80	187.0
105.90	482.0
106.90	158.0
108.00	113.0
111.00	124.0
111.70	120.0
112.10	111.0
113.00	142.0
115.00	158.0
115.90	443.0
116.90	938.0
117.90	400.0
118.90	845.0
123.90	143.0
126.10	123.0
127.90	302.0
129.00	251.0
129.90	422.0
130.80	218.0
135.00	302.0
137.00	321.0
140.10	124.0
141.00	980.0
142.10	210.0
142.90	1769.0
143.90	160.0
144.80	611.0
145.90	314.0
147.80	237.0
148.80	113.0
149.90	131.0
152.90	178.0
154.80	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

156.80	230.0
158.80	114.0
160.90	209.0
171.00	402.0
172.00	1148.0
174.00	92928.0
175.00	7297.0
176.00	89472.0
177.00	6341.0
178.00	221.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.20	156.0
36.00	1205.0
37.00	5207.0
38.10	5051.0
39.10	1990.0
39.90	319.0
42.50	217.0
43.00	174.0
44.10	816.0
45.00	1020.0
46.00	269.0
47.00	1409.0
48.10	781.0
49.00	4673.0
50.10	19536.0
51.10	6079.0
52.00	329.0
53.00	242.0
53.90	155.0
55.00	401.0
56.10	1440.0
57.00	2840.0
57.90	196.0
60.00	1219.0
61.00	4933.0
62.10	5115.0
63.10	4457.0
64.10	802.0
65.00	920.0
65.90	182.0
67.10	354.0
68.00	10165.0
69.10	10449.0
70.10	886.0
72.00	587.0
73.00	4941.0
74.10	17040.0
75.10	51144.0
76.10	4109.0
76.90	695.0
78.10	576.0
79.00	4188.0
80.00	1050.0
80.90	4442.0
81.90	846.0
83.10	150.0
87.00	4346.0
88.00	4326.0
91.00	531.0
92.00	3082.0
93.00	4972.0
94.00	11834.0
95.10	98872.0
96.10	6654.0
97.00	204.0
102.80	144.0
103.90	655.0
104.90	160.0
105.90	514.0
106.90	165.0
110.80	120.0
111.10	123.0
111.80	111.0
113.00	145.0
114.90	143.0
115.90	502.0
116.90	972.0
117.90	401.0
118.90	915.0
124.00	128.0
126.10	144.0
127.90	324.0
128.90	233.0
130.00	496.0
130.80	198.0
134.90	314.0
137.00	309.0
140.10	115.0
141.00	974.0
142.10	172.0
142.90	1647.0
143.90	204.0
144.90	593.0
145.90	288.0
147.80	277.0
148.80	121.0
149.80	142.0
152.90	182.0
154.80	294.0
156.80	260.0
158.80	106.0
159.90	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

160.90	198.0
171.00	410.0
172.00	1201.0
174.00	93584.0
175.00	7256.0
176.00	90104.0
177.00	6255.0
178.00	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240