
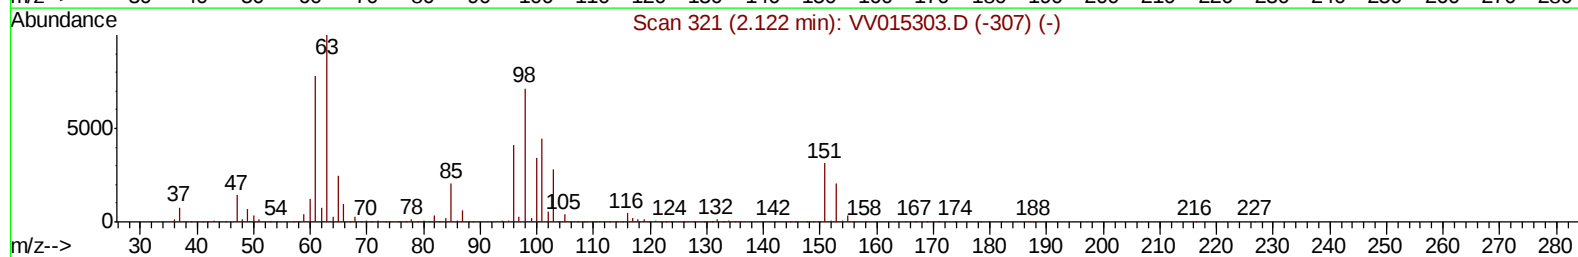
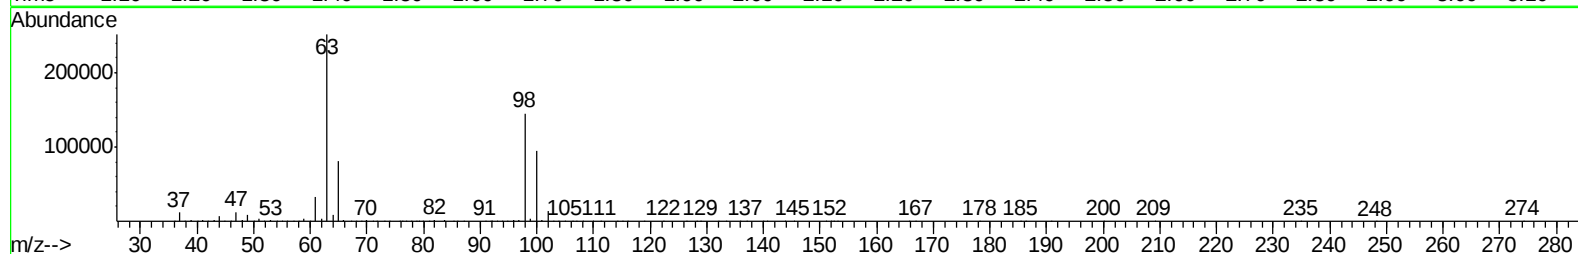


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015306.D
 Acq On : 31 Mar 2020 12:10
 Operator : SY/MD
 Sample : L1985-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 01:24:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 01 01:17:34 2020
 Response via : Initial Calibration

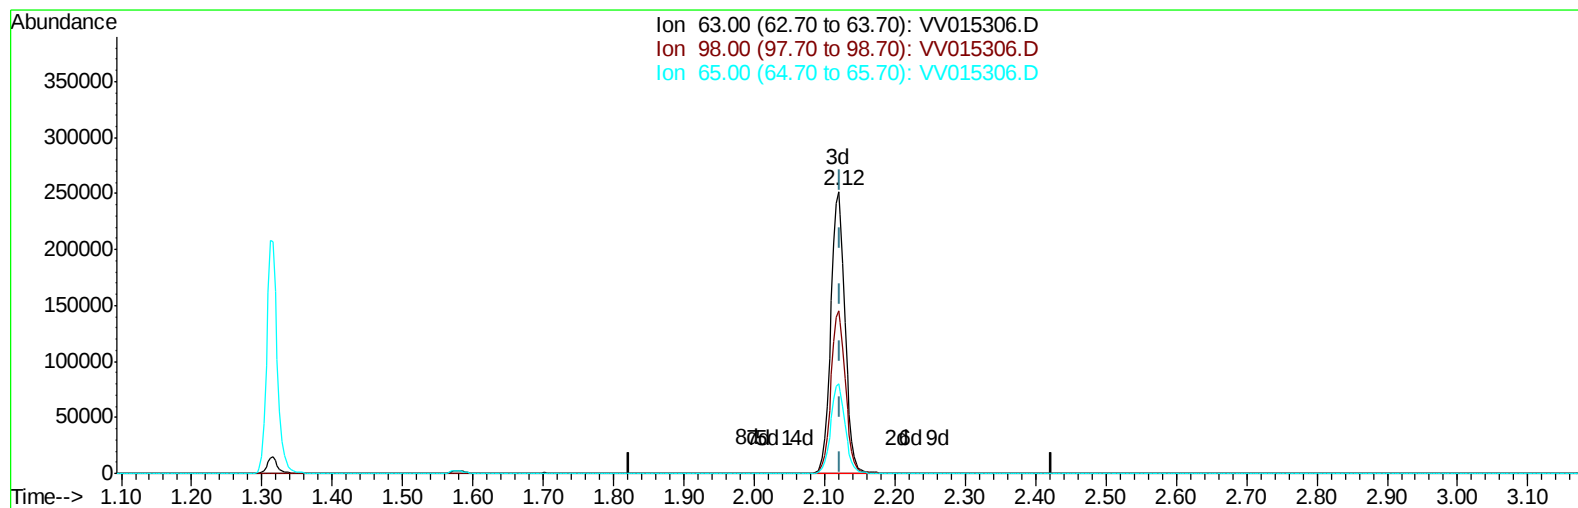

TIC: VV015306.D

(11) 1,1-Dichloroethene-d2 (S)

2.119min (-0.003) 53.80ug/L m

response 353091

Ion	Exp%	Act%
63.00	100	100
98.00	72.00	0.03#
65.00	23.00	0.01#
0.00	0.00	0.00