
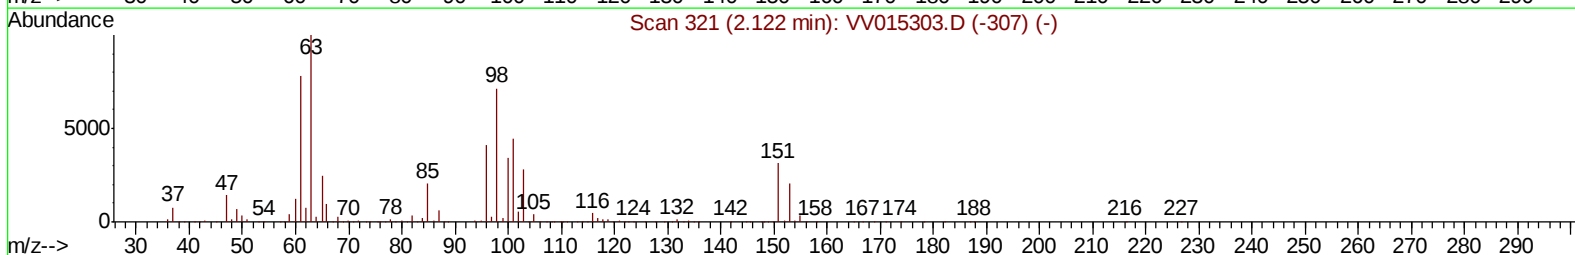
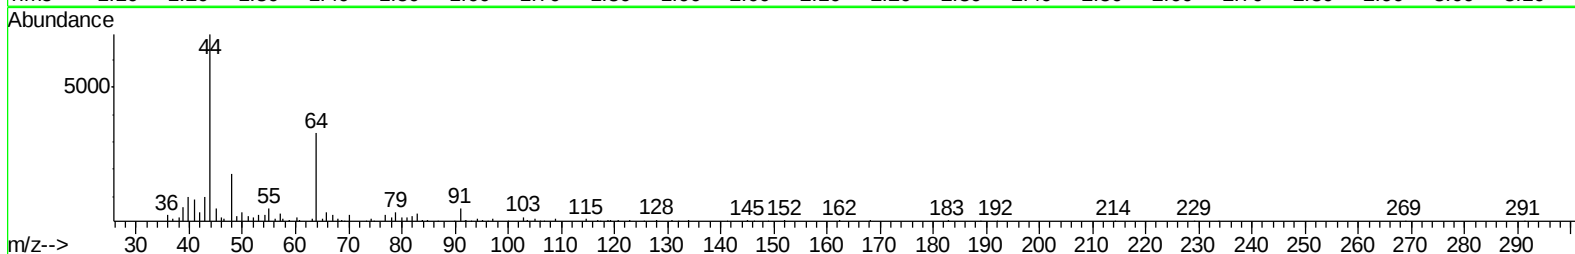


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV033120\
 Data File : VV015309.D
 Acq On : 31 Mar 2020 13:22
 Operator : SY/MD
 Sample : L1975-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 01:24:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 01 01:17:34 2020
 Response via : Initial Calibration

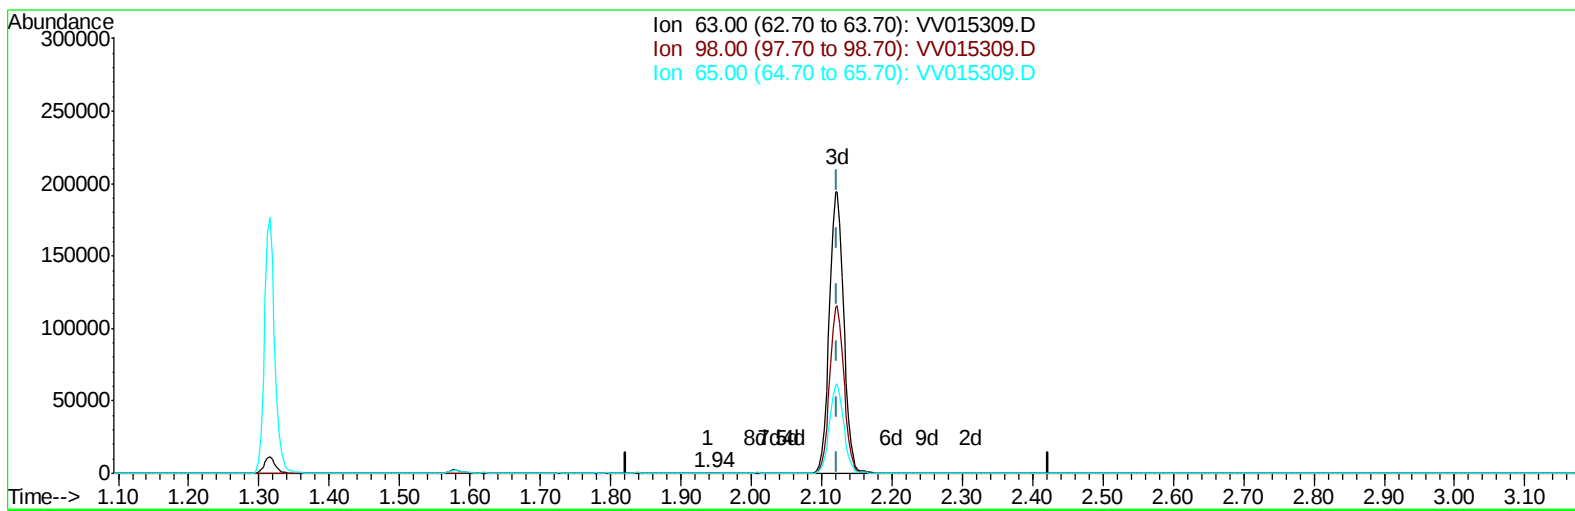

TIC: VV015309.D

(11) 1,1-Dichloroethene-d2 (S)

1.939min (-0.183) 0.02ug/L

response 149

Ion	Exp%	Act%
63.00	100	100
98.00	72.00	82.55
65.00	23.00	26.85
0.00	0.00	0.00