
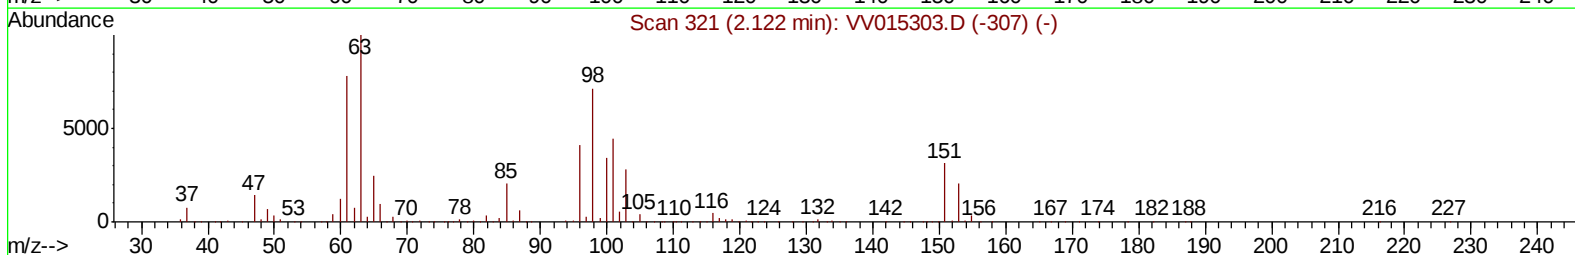
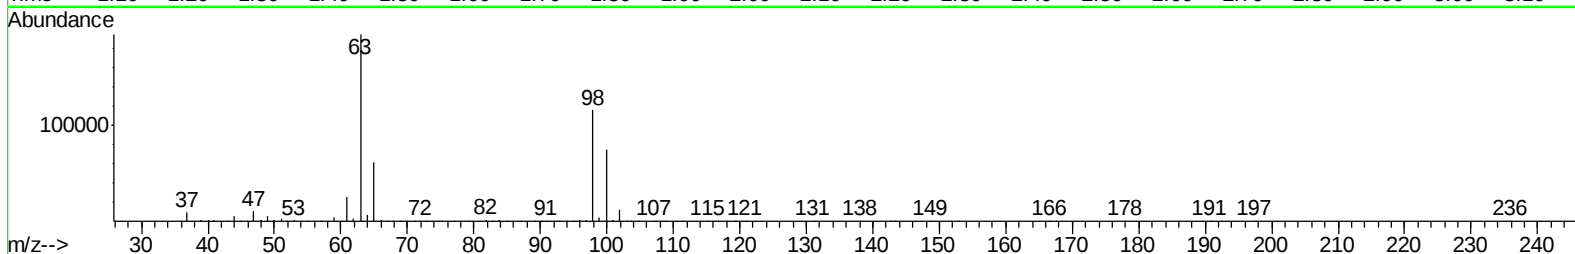


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV033120\  
 Data File : VV015309.D  
 Acq On : 31 Mar 2020 13:22  
 Operator : SY/MD  
 Sample : L1975-21  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 01:24:59 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM033020WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Apr 01 01:17:34 2020  
 Response via : Initial Calibration

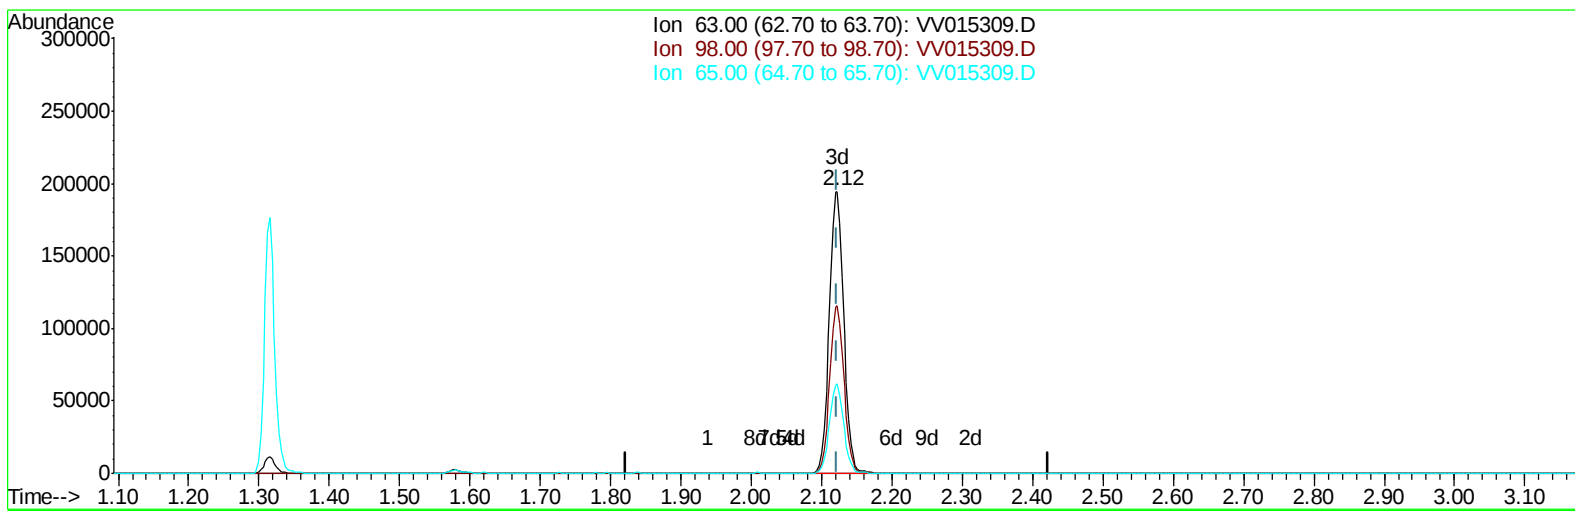

TIC: VV015309.D

(11) 1,1-Dichloroethene-d2 (S)

2.123min (+0.000) 38.03ug/L m

response 279500

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 63.00 | 100   | 100   |
| 98.00 | 72.00 | 0.04# |
| 65.00 | 23.00 | 0.01# |
| 0.00  | 0.00  | 0.00  |