
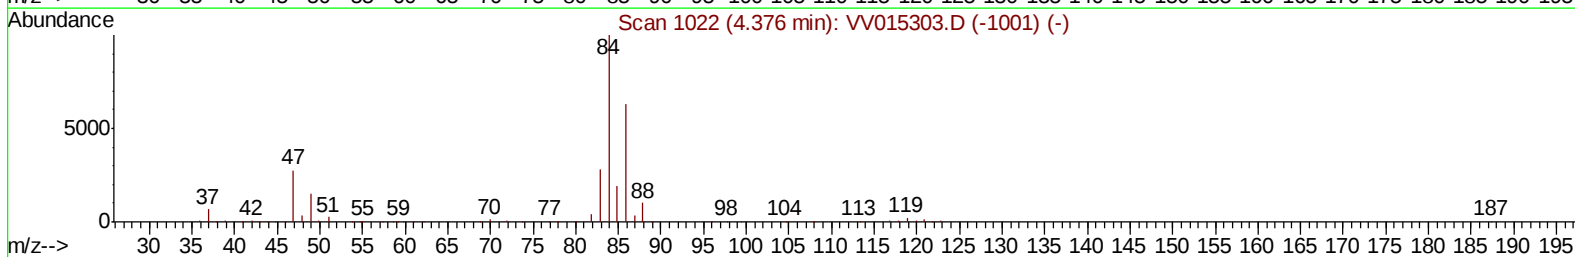
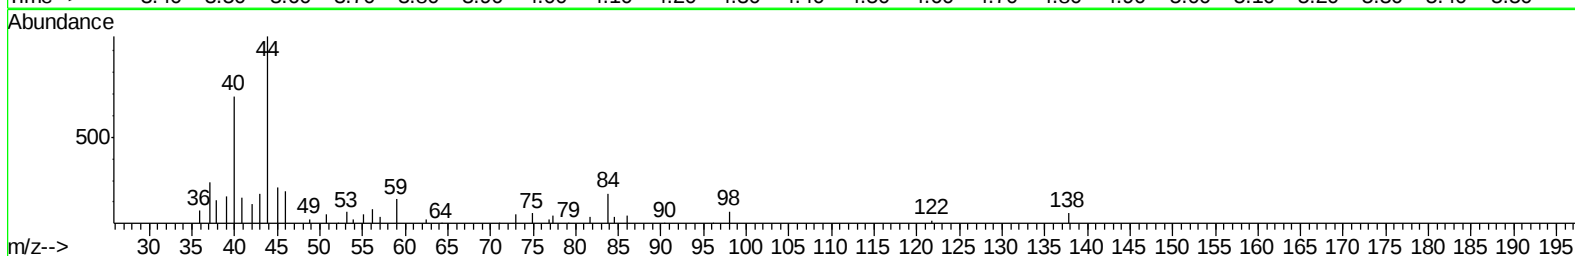


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015321.D
 Acq On : 31 Mar 2020 18:13
 Operator : SY/MD
 Sample : L1975-08 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 01:26:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 01 01:17:34 2020
 Response via : Initial Calibration

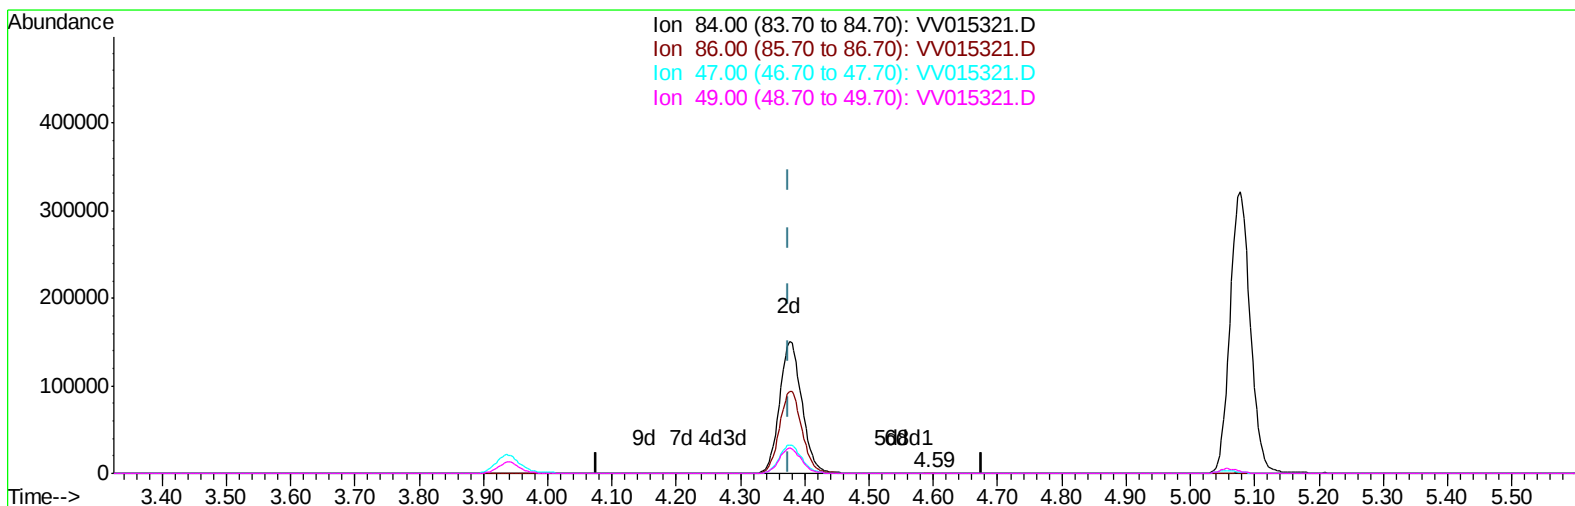

TIC: VV015321.D

(24) Chloroform-d (S)

4.592min (+0.215) 0.03ug/L

response 215

Ion	Exp%	Act%
84.00	100	100
86.00	61.40	51.63
47.00	42.50	39.53
49.00	26.20	21.40