
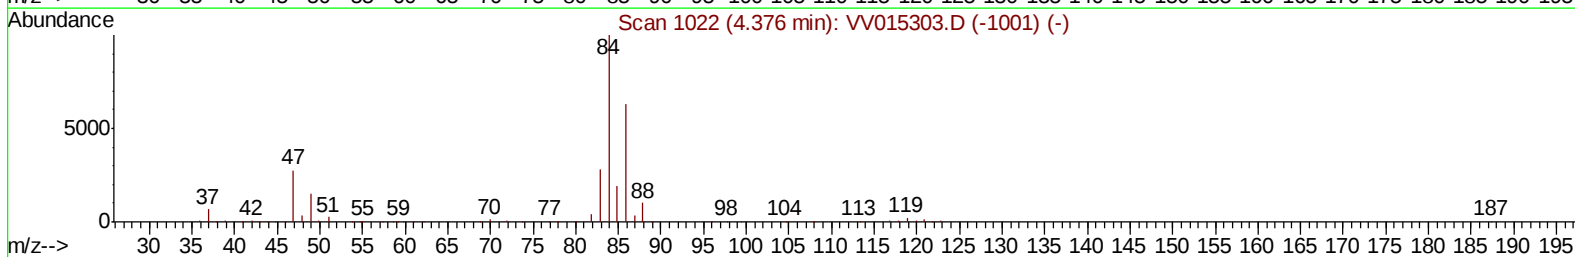
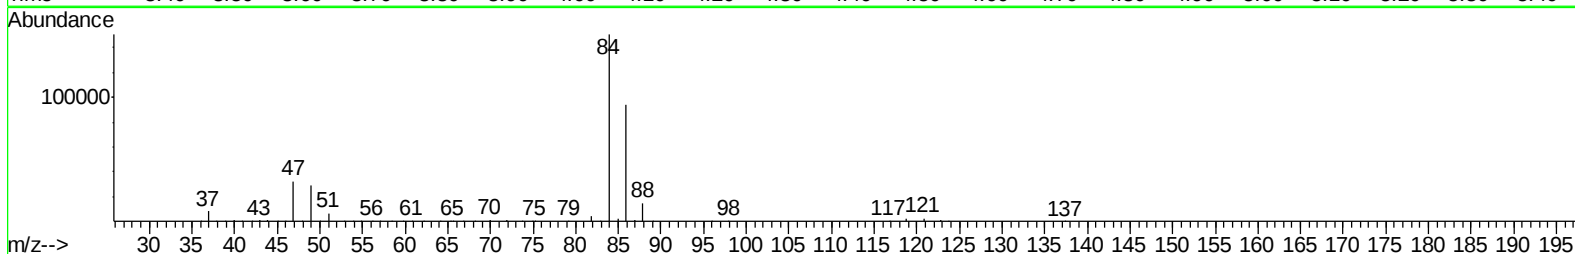


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015321.D
Acq On : 31 Mar 2020 18:13
Operator : SY/MD
Sample : L1975-08 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 01:26:52 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 01 01:17:34 2020
Response via : Initial Calibration

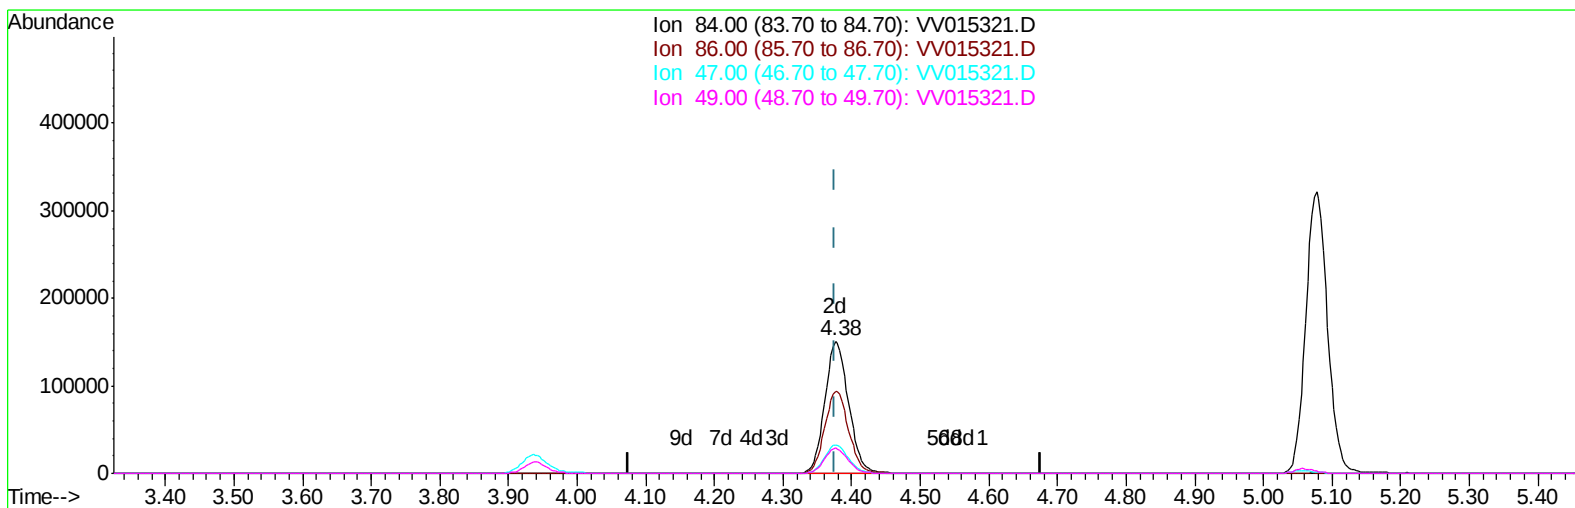

TIC: VV015321.D

(24) Chloroform-d (S)

4.376min (-0.000) 47.01ug/L m

response 361555

Ion	Exp%	Act%
84.00	100	100
86.00	61.40	0.03#
47.00	42.50	0.02#
49.00	26.20	0.01#