

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015305.D
 Acq On : 31 Mar 2020 11:45
 Operator : SY/MD
 Sample : L1985-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	292122	300366	15.01%	1.838%
2	1.576	146	151	164	rVB	256691	301873	15.09%	1.847%
3	2.119	312	320	337	rVB	577912	854240	42.69%	5.226%
4	2.910	564	566	568	rBV3	2092	1255	0.06%	0.008%
5	3.196	650	655	656	rBV4	2263	1923	0.10%	0.012%
6	3.248	668	671	672	rBV3	2931	1586	0.08%	0.010%
7	3.312	686	691	693	rBV6	3201	2386	0.12%	0.015%
8	3.383	710	713	717	rBV4	1436	1109	0.06%	0.007%
9	3.515	751	754	758	rBV6	1482	1087	0.05%	0.007%
10	3.534	758	760	762	rBV3	1618	839	0.04%	0.005%
11	3.598	777	780	781	rBV3	1494	929	0.05%	0.006%
12	3.653	793	797	802	rBV8	2768	2558	0.13%	0.016%
13	3.691	807	809	813	rVV3	1323	912	0.05%	0.006%
14	3.769	831	833	838	rVB5	1579	1087	0.05%	0.007%
15	3.804	842	844	850	rVB7	1996	1612	0.08%	0.010%
16	3.933	873	884	930	rBV2	99723	468225	23.40%	2.865%
17	4.373	1007	1021	1045	rVB2	323912	792802	39.62%	4.850%
18	4.756	1137	1140	1142	rBV4	1671	983	0.05%	0.006%
19	4.810	1155	1157	1162	rVB5	2240	1994	0.10%	0.012%
20	4.833	1162	1164	1167	rVB4	1714	1014	0.05%	0.006%
21	4.852	1167	1170	1175	rBV6	2694	2547	0.13%	0.016%
22	4.923	1189	1192	1195	rBV5	1852	1279	0.06%	0.008%
23	4.945	1195	1199	1203	rBV7	1605	1672	0.08%	0.010%
24	5.071	1218	1238	1264	rBV2	796135	2000868	100.00%	12.241%
25	5.540	1381	1384	1387	rBV5	1463	916	0.05%	0.006%
26	5.640	1402	1415	1442	rBV	663687	1321941	66.07%	8.088%
27	5.900	1492	1496	1497	rBV3	2989	2162	0.11%	0.013%
28	6.029	1533	1536	1539	rBV5	2080	1278	0.06%	0.008%
29	6.093	1542	1556	1576	rBV	451508	918750	45.92%	5.621%
30	6.367	1639	1641	1643	rBV3	1881	878	0.04%	0.005%
31	6.408	1651	1654	1655	rBV3	1689	940	0.05%	0.006%
32	6.437	1660	1663	1666	rBV4	1614	1161	0.06%	0.007%
33	6.711	1745	1748	1752	rVB6	1774	1428	0.07%	0.009%
34	6.791	1770	1773	1777	rBV5	1014	922	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015305.D
 Acq On : 31 Mar 2020 11:45
 Operator : SY/MD
 Sample : L1985-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	6.814	1777	1780	1783	rBV4	1474	976	0.05%	0.006%
36	7.006	1829	1840	1864	rBV	274470	492307	24.60%	3.012%
37	7.125	1875	1877	1880	rBV4	1439	868	0.04%	0.005%
38	7.206	1899	1902	1907	rBV5	2301	2046	0.10%	0.013%
39	7.338	1931	1943	1960	rBV	979395	1675625	83.74%	10.252%
40	7.582	2015	2019	2021	rBV4	2176	1488	0.07%	0.009%
41	7.643	2027	2038	2055	rBV	199087	342944	17.14%	2.098%
42	7.836	2095	2098	2102	rVB5	1706	1406	0.07%	0.009%
43	7.862	2102	2106	2108	rBV5	2461	1886	0.09%	0.012%
44	7.894	2114	2116	2121	rBV5	1137	1019	0.05%	0.006%
45	8.016	2152	2154	2157	rBV3	1416	1081	0.05%	0.007%
46	8.116	2172	2185	2210	rBV2	504990	1030508	51.50%	6.305%
47	8.875	2408	2421	2437	rBV	1032133	1664662	83.20%	10.184%
48	9.035	2464	2471	2474	rBV8	2797	3581	0.18%	0.022%
49	9.151	2501	2507	2508	rBV6	5181	4469	0.22%	0.027%
50	9.264	2539	2542	2545	rBV4	1830	1381	0.07%	0.008%
51	9.437	2594	2596	2598	rVV2	1314	830	0.04%	0.005%
52	9.566	2630	2636	2639	rBV7	4946	6374	0.32%	0.039%
53	9.659	2661	2665	2668	rBV5	1558	1274	0.06%	0.008%
54	9.813	2710	2713	2716	rVB5	1628	997	0.05%	0.006%
55	9.829	2716	2718	2725	rBV7	2631	3118	0.16%	0.019%
56	10.010	2771	2774	2776	rBV3	2043	1082	0.05%	0.007%
57	10.045	2779	2785	2787	rBV6	1883	1910	0.10%	0.012%
58	10.174	2822	2825	2830	rBV7	1369	1244	0.06%	0.008%
59	10.238	2832	2845	2865	rBV	608307	961725	48.07%	5.884%
60	10.370	2881	2886	2887	rBV4	2166	1505	0.08%	0.009%
61	10.469	2912	2917	2919	rBV5	2377	2180	0.11%	0.013%
62	10.540	2932	2939	2940	rBV5	1560	1367	0.07%	0.008%
63	10.736	2994	3000	3002	rBV7	1683	1725	0.09%	0.011%
64	10.823	3024	3027	3030	rVB5	1381	871	0.04%	0.005%
65	10.855	3034	3037	3039	rBV3	1949	1229	0.06%	0.008%
66	10.878	3042	3044	3049	rVV5	1503	1137	0.06%	0.007%
67	11.067	3101	3103	3108	rBV7	1559	852	0.04%	0.005%
68	11.119	3115	3119	3120	rBV4	1437	973	0.05%	0.006%
69	11.148	3126	3128	3131	rVB4	2152	959	0.05%	0.006%
70	11.186	3137	3140	3141	rBV3	2232	1456	0.07%	0.009%
71	11.273	3155	3167	3190	rBV	1017356	1566524	78.29%	9.584%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015305.D
 Acq On : 31 Mar 2020 11:45
 Operator : SY/MD
 Sample : L1985-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	11.485	3230	3233	3235	rBV4	1509	952	0.05%	0.006%
73	11.559	3248	3256	3267	rBV2	27530	45464	2.27%	0.278%
74	11.646	3272	3283	3303	rVV	943854	1473208	73.63%	9.013%
75	11.871	3352	3353	3356	rVB3	2150	936	0.05%	0.006%
76	11.890	3356	3359	3361	rVB3	1843	849	0.04%	0.005%
77	11.913	3361	3366	3368	rBV4	2207	1752	0.09%	0.011%
78	11.932	3368	3372	3374	rBV4	2359	1850	0.09%	0.011%
79	12.038	3402	3405	3407	rBV4	2508	1505	0.08%	0.009%
80	12.109	3424	3427	3429	rVB2	2136	1250	0.06%	0.008%
81	12.128	3429	3433	3434	rBV3	1775	943	0.05%	0.006%
82	12.225	3458	3463	3465	rBV5	1051	987	0.05%	0.006%
83	12.331	3494	3496	3498	rBV3	2284	1268	0.06%	0.008%
84	12.678	3601	3604	3611	rVB8	3570	3336	0.17%	0.020%
85	12.772	3631	3633	3636	rVV3	1944	928	0.05%	0.006%
86	12.807	3640	3644	3649	rVB6	2617	2145	0.11%	0.013%
87	12.913	3671	3677	3680	rBV7	2633	3028	0.15%	0.019%
88	12.964	3688	3693	3697	rBV8	1893	1543	0.08%	0.009%
89	13.151	3748	3751	3754	rVB4	1581	1059	0.05%	0.006%
90	13.321	3801	3804	3809	rVB7	2020	1821	0.09%	0.011%
91	13.434	3836	3839	3843	rBV5	1648	1029	0.05%	0.006%
92	13.489	3852	3856	3858	rBV5	1240	1038	0.05%	0.006%
93	13.530	3861	3869	3871	rBV8	5458	7271	0.36%	0.044%
94	13.714	3923	3926	3930	rBV4	1350	996	0.05%	0.006%
95	13.935	3992	3995	3996	rBV3	1675	1016	0.05%	0.006%
96	13.997	4013	4014	4017	rBV3	1822	860	0.04%	0.005%
97	14.215	4078	4082	4084	rBV5	1786	1381	0.07%	0.008%
98	14.244	4088	4091	4096	rVV5	1614	1285	0.06%	0.008%
99	14.707	4232	4235	4239	rBV6	2651	2404	0.12%	0.015%
100	14.826	4270	4272	4276	rBV4	2231	1910	0.10%	0.012%


Sum of corrected areas: 16345115

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015305.D
Acq On : 31 Mar 2020 11:45
Operator : SY/MD
Sample : L1985-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

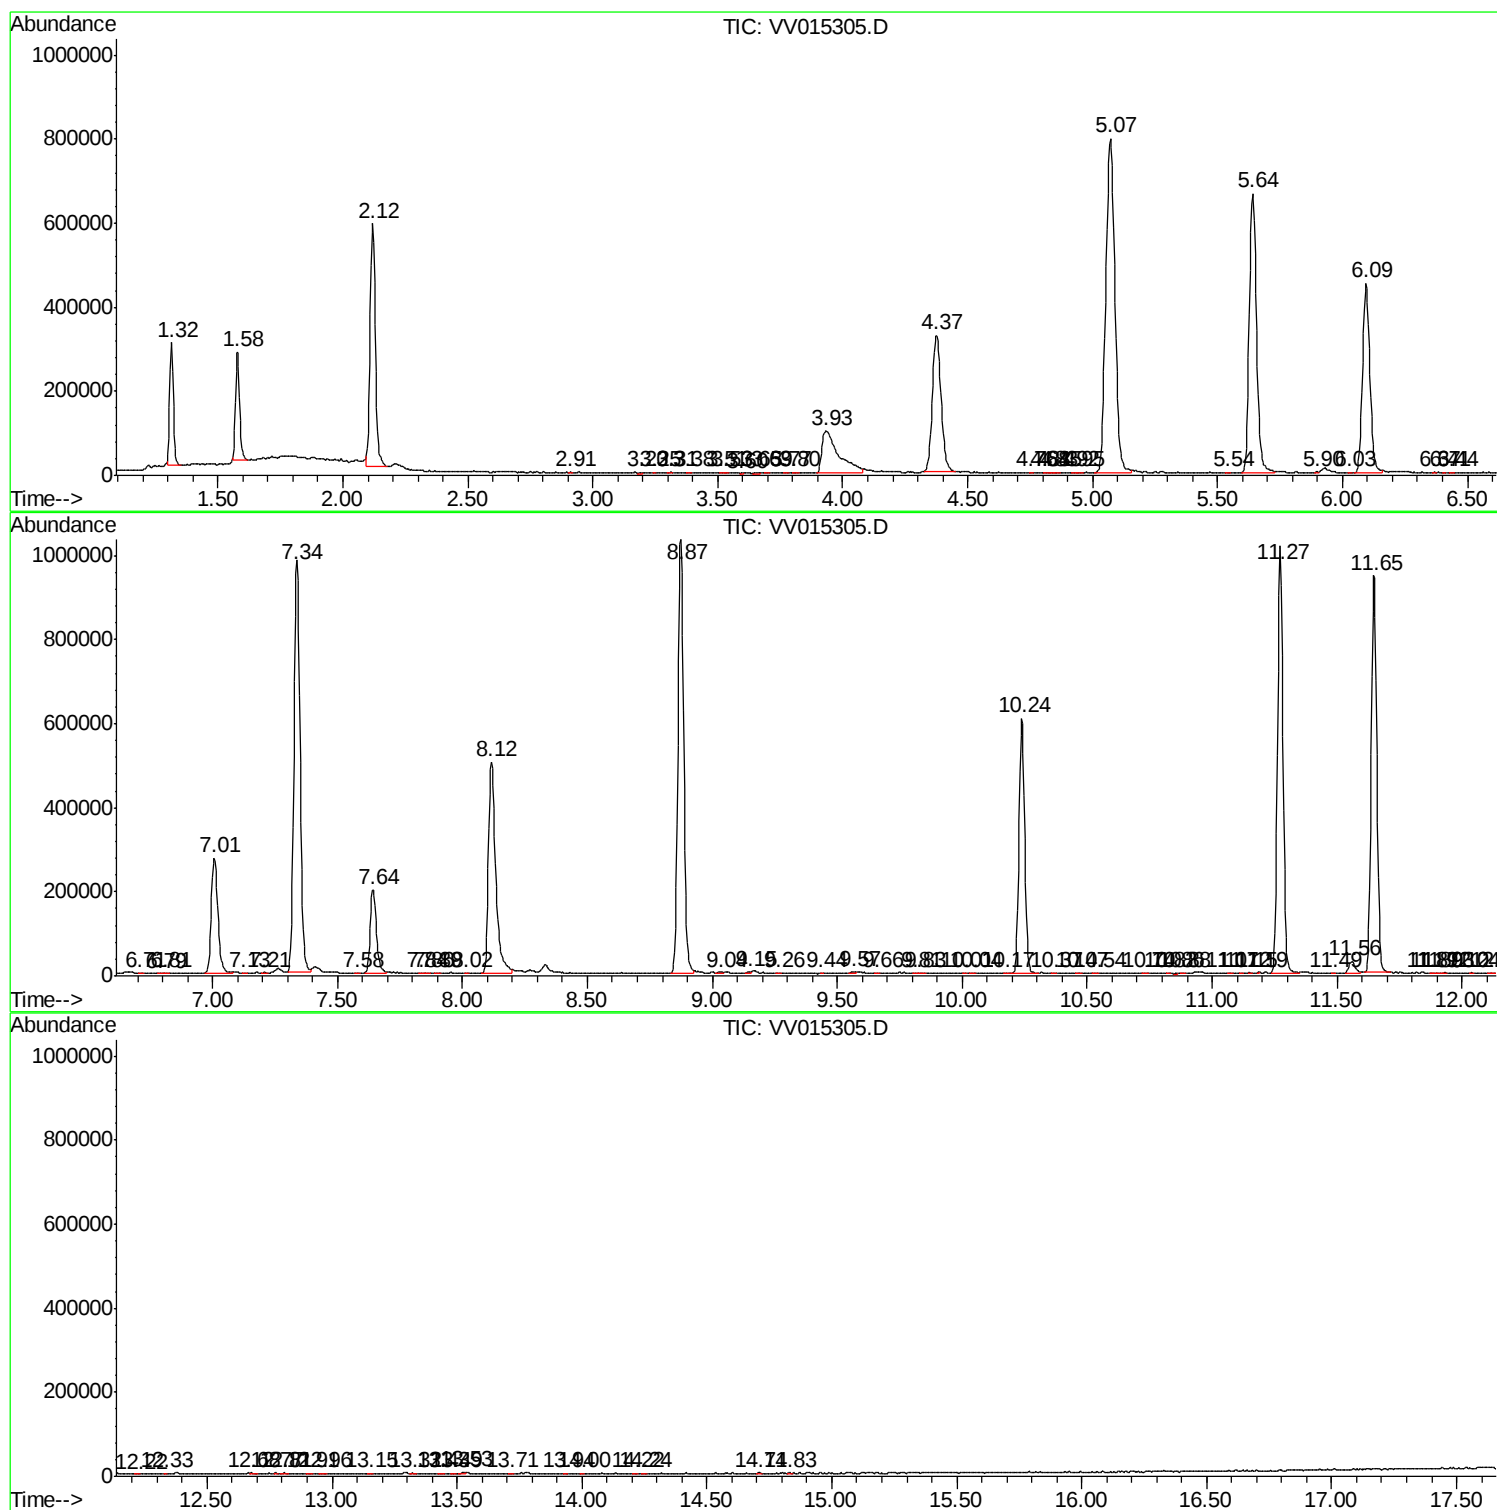

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015305.D
Acq On : 31 Mar 2020 11:45
Operator : SY/MD
Sample : L1985-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015305.D
Acq On : 31 Mar 2020 11:45
Operator : SY/MD
Sample : L1985-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc