

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015316.D
 Acq On : 31 Mar 2020 16:12
 Operator : SY/MD
 Sample : L1975-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	89	rVB2	1549199	1662349	73.42%	7.984%
2	1.579	146	152	166	rBV	277960	337976	14.93%	1.623%
3	2.119	313	320	340	rVB	589649	866074	38.25%	4.160%
4	2.666	487	490	494	rVB6	2780	1491	0.07%	0.007%
5	2.688	494	497	499	rBV4	1939	1292	0.06%	0.006%
6	2.782	517	526	539	rVB	61907	108208	4.78%	0.520%
7	2.929	568	572	574	rBV5	1737	1200	0.05%	0.006%
8	2.958	575	581	582	rBV6	3081	2453	0.11%	0.012%
9	3.048	606	609	612	rBV4	1556	1134	0.05%	0.005%
10	3.216	657	661	667	rVB7	2534	2577	0.11%	0.012%
11	3.290	682	684	685	rBV2	1483	783	0.03%	0.004%
12	3.405	717	720	723	rBV3	1838	1266	0.06%	0.006%
13	3.450	728	734	738	rBV9	1854	1970	0.09%	0.009%
14	3.473	740	741	742	rBV2	1024	253	0.01%	0.001%
15	3.515	752	754	756	rVB3	1674	753	0.03%	0.004%
16	3.527	756	758	761	rVB4	1038	470	0.02%	0.002%
17	3.544	761	763	767	rBV4	1891	1443	0.06%	0.007%
18	3.605	780	782	786	rVB4	874	528	0.02%	0.003%
19	3.627	786	789	790	rBV3	1473	789	0.03%	0.004%
20	3.656	796	798	799	rBV2	725	348	0.02%	0.002%
21	3.666	799	801	802	rVB2	1185	344	0.02%	0.002%
22	3.675	802	804	807	rBV4	1209	668	0.03%	0.003%
23	3.691	807	809	811	rBV3	1428	682	0.03%	0.003%
24	3.704	811	813	816	rVV4	1262	713	0.03%	0.003%
25	3.730	819	821	822	rBV2	1210	525	0.02%	0.003%
26	3.939	871	886	921	rBV2	862021	2264315	100.00%	10.875%
27	4.376	1008	1022	1049	rVB	352886	856739	37.84%	4.115%
28	4.601	1090	1092	1096	rBV5	1643	1337	0.06%	0.006%
29	4.659	1108	1110	1114	rBV5	2220	1836	0.08%	0.009%
30	4.775	1144	1146	1148	rVB3	1427	589	0.03%	0.003%
31	4.798	1150	1153	1157	rVV4	1878	1253	0.06%	0.006%
32	4.910	1187	1188	1190	rBV2	1098	549	0.02%	0.003%
33	4.971	1204	1207	1210	rBV5	1246	806	0.04%	0.004%
34	5.074	1223	1239	1267	rBV2	847089	2120050	93.63%	10.183%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015316.D
 Acq On : 31 Mar 2020 16:12
 Operator : SY/MD
 Sample : L1975-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	5.563	1385	1391	1393	rBV4	7410	7200	0.32%	0.035%
36	5.643	1404	1416	1435	rBV	672251	1336843	59.04%	6.421%
37	6.096	1544	1557	1578	rBV	485382	982074	43.37%	4.717%
38	6.923	1811	1814	1818	rBV5	1898	1547	0.07%	0.007%
39	6.942	1818	1820	1823	rBV4	1268	965	0.04%	0.005%
40	7.006	1829	1840	1859	rBV	296167	532938	23.54%	2.560%
41	7.338	1931	1943	1961	rBV	1031734	1792961	79.18%	8.612%
42	7.643	2028	2038	2059	rBV	215038	359744	15.89%	1.728%
43	7.945	2131	2132	2133	rBV	962	268	0.01%	0.001%
44	8.112	2173	2184	2218	rBV	764293	1438025	63.51%	6.907%
45	8.620	2339	2342	2343	rBV3	1885	1078	0.05%	0.005%
46	8.875	2409	2421	2438	rBV	1084995	1750641	77.31%	8.408%
47	9.547	2627	2630	2631	rBV3	2171	1238	0.05%	0.006%
48	9.672	2667	2669	2672	rBV4	1683	1143	0.05%	0.005%
49	9.730	2683	2687	2689	rBV4	6546	5472	0.24%	0.026%
50	10.238	2834	2845	2862	rBV	711599	1118127	49.38%	5.370%
51	10.450	2908	2911	2915	rBV6	2867	2786	0.12%	0.013%
52	10.707	2987	2991	2993	rBV4	3107	2655	0.12%	0.013%
53	10.871	3040	3042	3047	rBV6	2284	1800	0.08%	0.009%
54	11.273	3155	3167	3187	rBV	1060502	1617157	71.42%	7.767%
55	11.649	3273	3284	3304	rVB	1038740	1615124	71.33%	7.757%
56	12.653	3594	3596	3597	rBV3	1613	666	0.03%	0.003%
57	12.726	3618	3619	3621	rVB2	1218	371	0.02%	0.002%
58	13.562	3877	3879	3884	rBV6	1934	1674	0.07%	0.008%
59	13.749	3935	3937	3940	rBV4	1982	1272	0.06%	0.006%
60	13.836	3962	3964	3967	rVB5	2210	806	0.04%	0.004%
61	14.662	4219	4221	4223	rBV3	2043	963	0.04%	0.005%
62	14.752	4247	4249	4251	rBV3	2496	1224	0.05%	0.006%


Sum of corrected areas: 20820525

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015316.D
Acq On : 31 Mar 2020 16:12
Operator : SY/MD
Sample : L1975-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

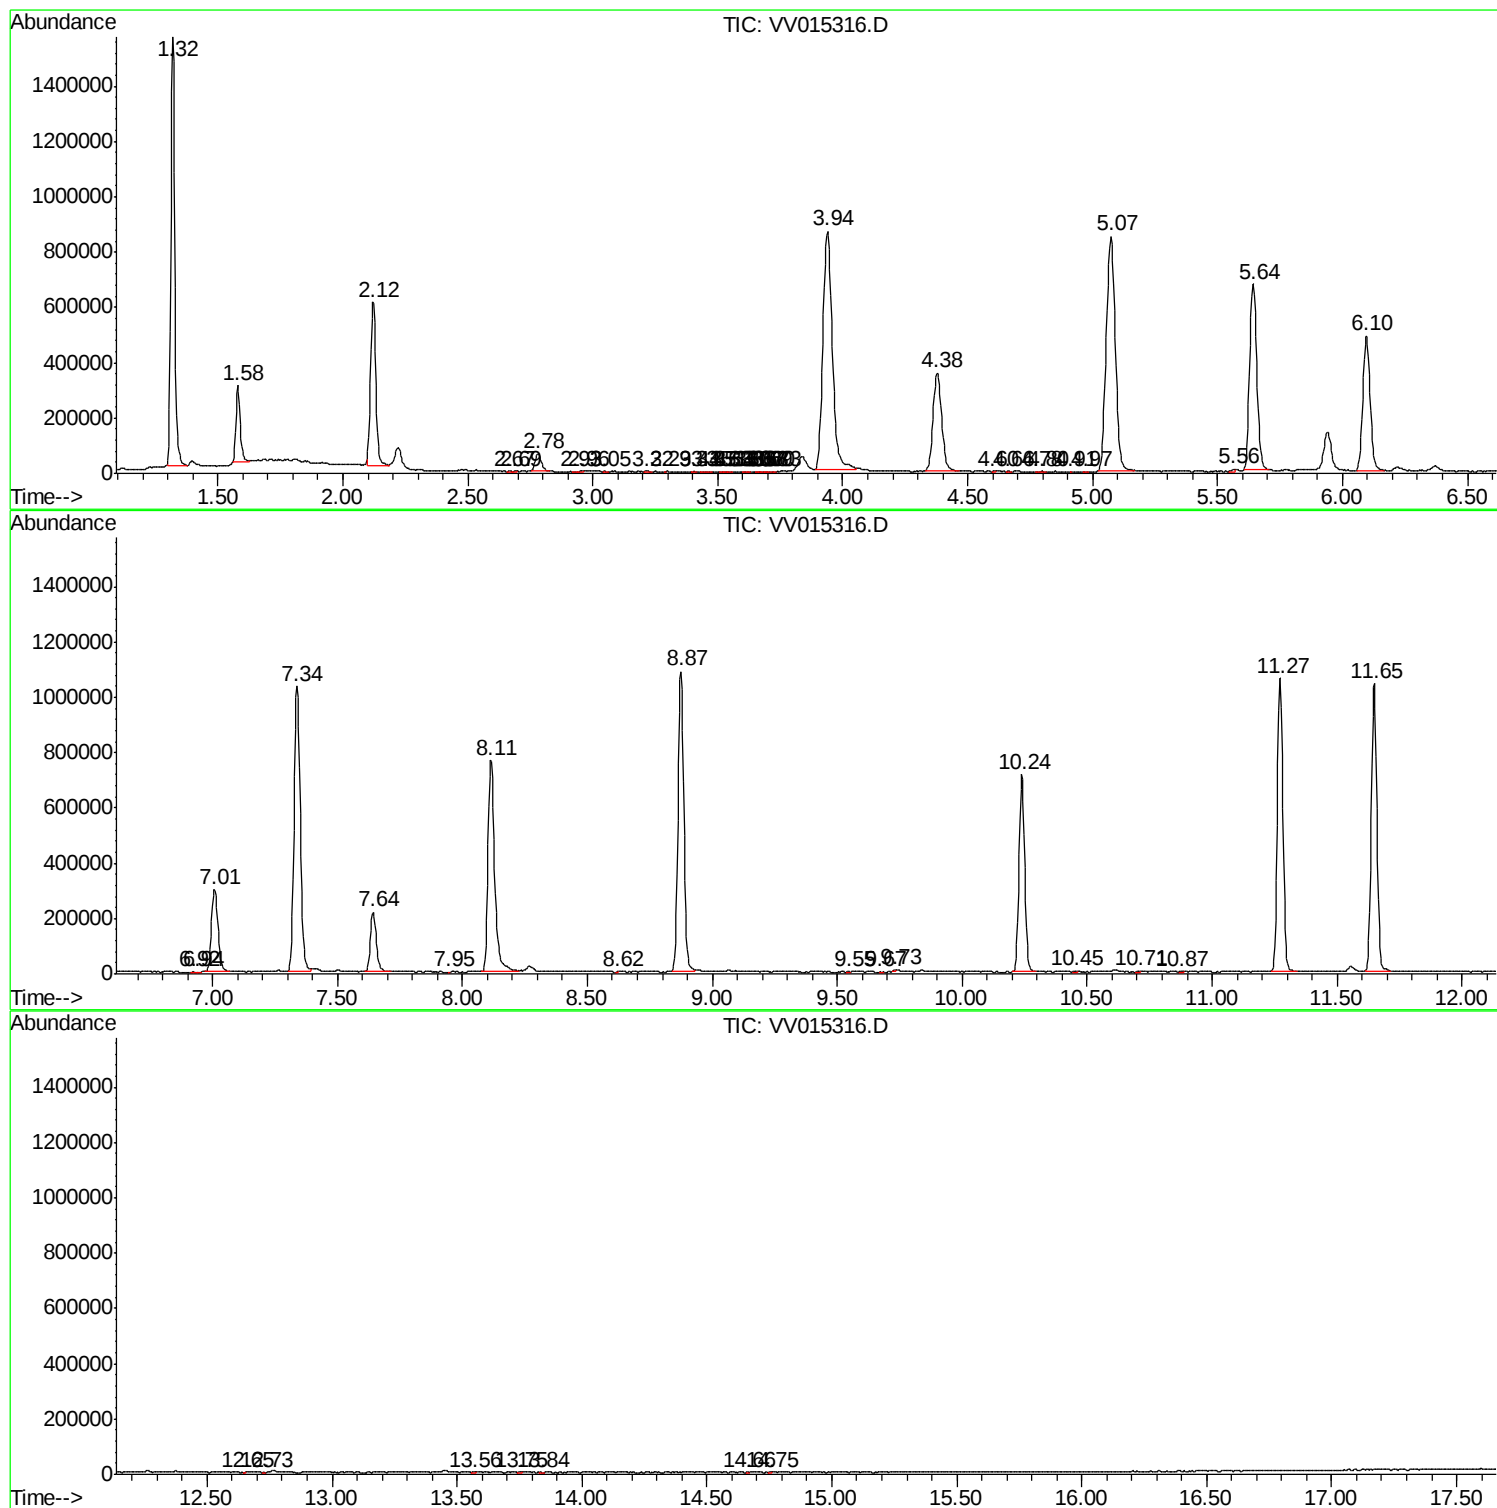

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015316.D
Acq On : 31 Mar 2020 16:12
Operator : SY/MD
Sample : L1975-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015316.D
Acq On : 31 Mar 2020 16:12
Operator : SY/MD
Sample : L1975-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc