

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015317.D
 Acq On : 31 Mar 2020 16:36
 Operator : SY/MD
 Sample : VIBLK88
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	296645	312623	14.25%	1.777%
2	1.579	146	152	164	rVB	281670	330267	15.06%	1.878%
3	2.119	312	320	338	rVB	600533	892011	40.66%	5.071%
4	2.891	558	560	564	rVB3	2206	1024	0.05%	0.006%
5	3.068	612	615	616	rBV3	2056	1260	0.06%	0.007%
6	3.222	660	663	664	rBV3	1608	857	0.04%	0.005%
7	3.232	664	666	670	rVB4	2360	1215	0.06%	0.007%
8	3.248	670	671	673	rBV2	1079	607	0.03%	0.003%
9	3.303	685	688	691	rBV4	1551	1161	0.05%	0.007%
10	3.341	697	700	702	rBV3	1362	866	0.04%	0.005%
11	3.376	709	711	713	rBV4	1401	781	0.04%	0.004%
12	3.495	746	748	750	rBV3	1147	651	0.03%	0.004%
13	3.531	756	759	761	rBV4	1480	709	0.03%	0.004%
14	3.576	771	773	774	rBV	1119	591	0.03%	0.003%
15	3.647	791	795	796	rBV4	2058	1290	0.06%	0.007%
16	3.688	805	808	812	rBV6	1898	1445	0.07%	0.008%
17	3.740	818	824	826	rBV6	2269	2507	0.11%	0.014%
18	3.782	835	837	840	rVB3	829	365	0.02%	0.002%
19	3.801	840	843	846	rBV5	1789	1233	0.06%	0.007%
20	3.823	846	850	855	rVB7	1757	1567	0.07%	0.009%
21	3.849	855	858	863	rBV7	1320	1283	0.06%	0.007%
22	3.872	863	865	868	rBV3	1146	825	0.04%	0.005%
23	3.926	871	882	912	rBV	137508	467731	21.32%	2.659%
24	4.296	994	997	998	rBV3	2209	1206	0.05%	0.007%
25	4.376	1008	1022	1046	rVB	357265	865347	39.45%	4.920%
26	4.566	1079	1081	1084	rBV4	1043	547	0.02%	0.003%
27	4.675	1113	1115	1117	rBV3	1565	629	0.03%	0.004%
28	4.872	1175	1176	1179	rVB3	967	381	0.02%	0.002%
29	4.891	1179	1182	1183	rBV3	1278	629	0.03%	0.004%
30	4.907	1183	1187	1191	rVB7	2256	1575	0.07%	0.009%
31	4.946	1191	1199	1201	rBV9	2214	2207	0.10%	0.013%
32	5.010	1216	1219	1221	rBV4	1945	1102	0.05%	0.006%
33	5.071	1221	1238	1264	rVV2	865622	2193707	100.00%	12.472%
34	5.283	1302	1304	1308	rVB5	2475	1318	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015317.D
 Acq On : 31 Mar 2020 16:36
 Operator : SY/MD
 Sample : VIBLK88
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	5.392	1336	1338	1339	rBV2	1471	514	0.02%	0.003%
36	5.495	1367	1370	1373	rBV4	1920	1850	0.08%	0.011%
37	5.534	1380	1382	1385	rVB4	2560	1155	0.05%	0.007%
38	5.576	1393	1395	1398	rBV4	1669	839	0.04%	0.005%
39	5.640	1402	1415	1441	rBV	699512	1414239	64.47%	8.040%
40	6.093	1545	1556	1575	rVB2	490328	981268	44.73%	5.579%
41	7.007	1829	1840	1860	rBV	301472	534455	24.36%	3.038%
42	7.338	1931	1943	1965	rBV	1052720	1819514	82.94%	10.344%
43	7.588	2018	2021	2022	rBV3	1625	971	0.04%	0.006%
44	7.643	2028	2038	2053	rBV	211877	351438	16.02%	1.998%
45	8.068	2168	2170	2173	rBV3	1469	914	0.04%	0.005%
46	8.113	2173	2184	2212	rBV	636650	1190620	54.27%	6.769%
47	8.775	2386	2390	2400	rVB	2779	3962	0.18%	0.023%
48	8.823	2402	2405	2406	rBV3	1611	1025	0.05%	0.006%
49	8.875	2408	2421	2443	rBV	1118464	1779755	81.13%	10.118%
50	9.386	2577	2580	2582	rBV3	1133	700	0.03%	0.004%
51	9.415	2587	2589	2593	rBV5	2050	1421	0.06%	0.008%
52	9.460	2600	2603	2606	rBV4	1963	1651	0.08%	0.009%
53	9.797	2706	2708	2710	rBV2	1086	542	0.02%	0.003%
54	9.926	2741	2748	2750	rBV7	1919	2189	0.10%	0.012%
55	10.148	2814	2817	2822	rBV5	1446	1079	0.05%	0.006%
56	10.238	2831	2845	2864	rBV	687266	1087218	49.56%	6.181%
57	10.386	2885	2891	2892	rBV5	2190	1716	0.08%	0.010%
58	10.518	2931	2932	2934	rBV2	1511	602	0.03%	0.003%
59	10.556	2941	2944	2946	rBV3	1143	605	0.03%	0.003%
60	10.633	2966	2968	2971	rVB4	1511	808	0.04%	0.005%
61	10.675	2978	2981	2982	rBV3	1826	1002	0.05%	0.006%
62	10.842	3032	3033	3038	rVB4	2026	1497	0.07%	0.009%
63	10.865	3038	3040	3041	rBV2	1834	779	0.04%	0.004%
64	10.875	3041	3043	3046	rVV4	1725	935	0.04%	0.005%
65	11.029	3089	3091	3094	rVB3	1616	892	0.04%	0.005%
66	11.096	3109	3112	3115	rVB5	1724	1023	0.05%	0.006%
67	11.116	3115	3118	3123	rBV6	2537	1800	0.08%	0.010%
68	11.270	3154	3166	3188	rBV	1082405	1642353	74.87%	9.337%
69	11.559	3248	3256	3260	rBV9	4564	6798	0.31%	0.039%
70	11.646	3271	3283	3304	rBV	1051463	1623955	74.03%	9.233%
71	11.981	3385	3387	3388	rBV2	1336	442	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015317.D
 Acq On : 31 Mar 2020 16:36
 Operator : SY/MD
 Sample : VIBLK88
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

72	12.035	3402	3404	3407	rVB4	1342	462	0.02%	0.003%
73	12.058	3409	3411	3412	rBV2	1498	736	0.03%	0.004%
74	12.106	3423	3426	3430	rVB6	1462	1330	0.06%	0.008%
75	12.132	3430	3434	3437	rBV5	1392	1091	0.05%	0.006%
76	12.145	3437	3438	3440	rBV	899	505	0.02%	0.003%
77	12.238	3463	3467	3469	rBV5	1258	1160	0.05%	0.007%
78	12.338	3495	3498	3501	rBV5	1926	1279	0.06%	0.007%
79	12.447	3529	3532	3534	rBV3	3313	2006	0.09%	0.011%
80	12.595	3575	3578	3583	rVB6	2653	2700	0.12%	0.015%
81	12.617	3583	3585	3589	rBV4	1551	1332	0.06%	0.008%
82	12.694	3606	3609	3612	rBV5	1948	1202	0.05%	0.007%
83	12.736	3620	3622	3624	rBV3	1453	763	0.03%	0.004%
84	12.807	3642	3644	3647	rBV4	2139	1414	0.06%	0.008%
85	13.125	3736	3743	3746	rBV7	2548	2901	0.13%	0.016%
86	13.222	3770	3773	3776	rBV4	1726	1226	0.06%	0.007%
87	13.318	3800	3803	3806	rBV5	1675	1344	0.06%	0.008%
88	13.386	3822	3824	3827	rVB4	1402	624	0.03%	0.004%
89	13.440	3838	3841	3842	rBV2	1592	927	0.04%	0.005%
90	13.460	3845	3847	3850	rVB4	1964	1036	0.05%	0.006%
91	13.479	3850	3853	3857	rBV5	2108	1787	0.08%	0.010%
92	13.772	3940	3944	3947	rBV6	2585	2168	0.10%	0.012%
93	13.813	3955	3957	3959	rBV3	1495	606	0.03%	0.003%
94	13.939	3994	3996	3998	rBV3	891	445	0.02%	0.003%
95	14.006	4014	4017	4020	rBV4	1423	1297	0.06%	0.007%
96	14.109	4047	4049	4050	rBV2	1173	327	0.01%	0.002%
97	14.585	4194	4197	4198	rBV3	1589	804	0.04%	0.005%
98	14.701	4231	4233	4236	rBV4	1431	939	0.04%	0.005%
99	14.993	4322	4324	4326	rBV3	2089	898	0.04%	0.005%
100	15.447	4463	4465	4468	rBV4	2668	2189	0.10%	0.012%


Sum of corrected areas: 17589541

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015317.D
Acq On : 31 Mar 2020 16:36
Operator : SY/MD
Sample : VIBLK88
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK88

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

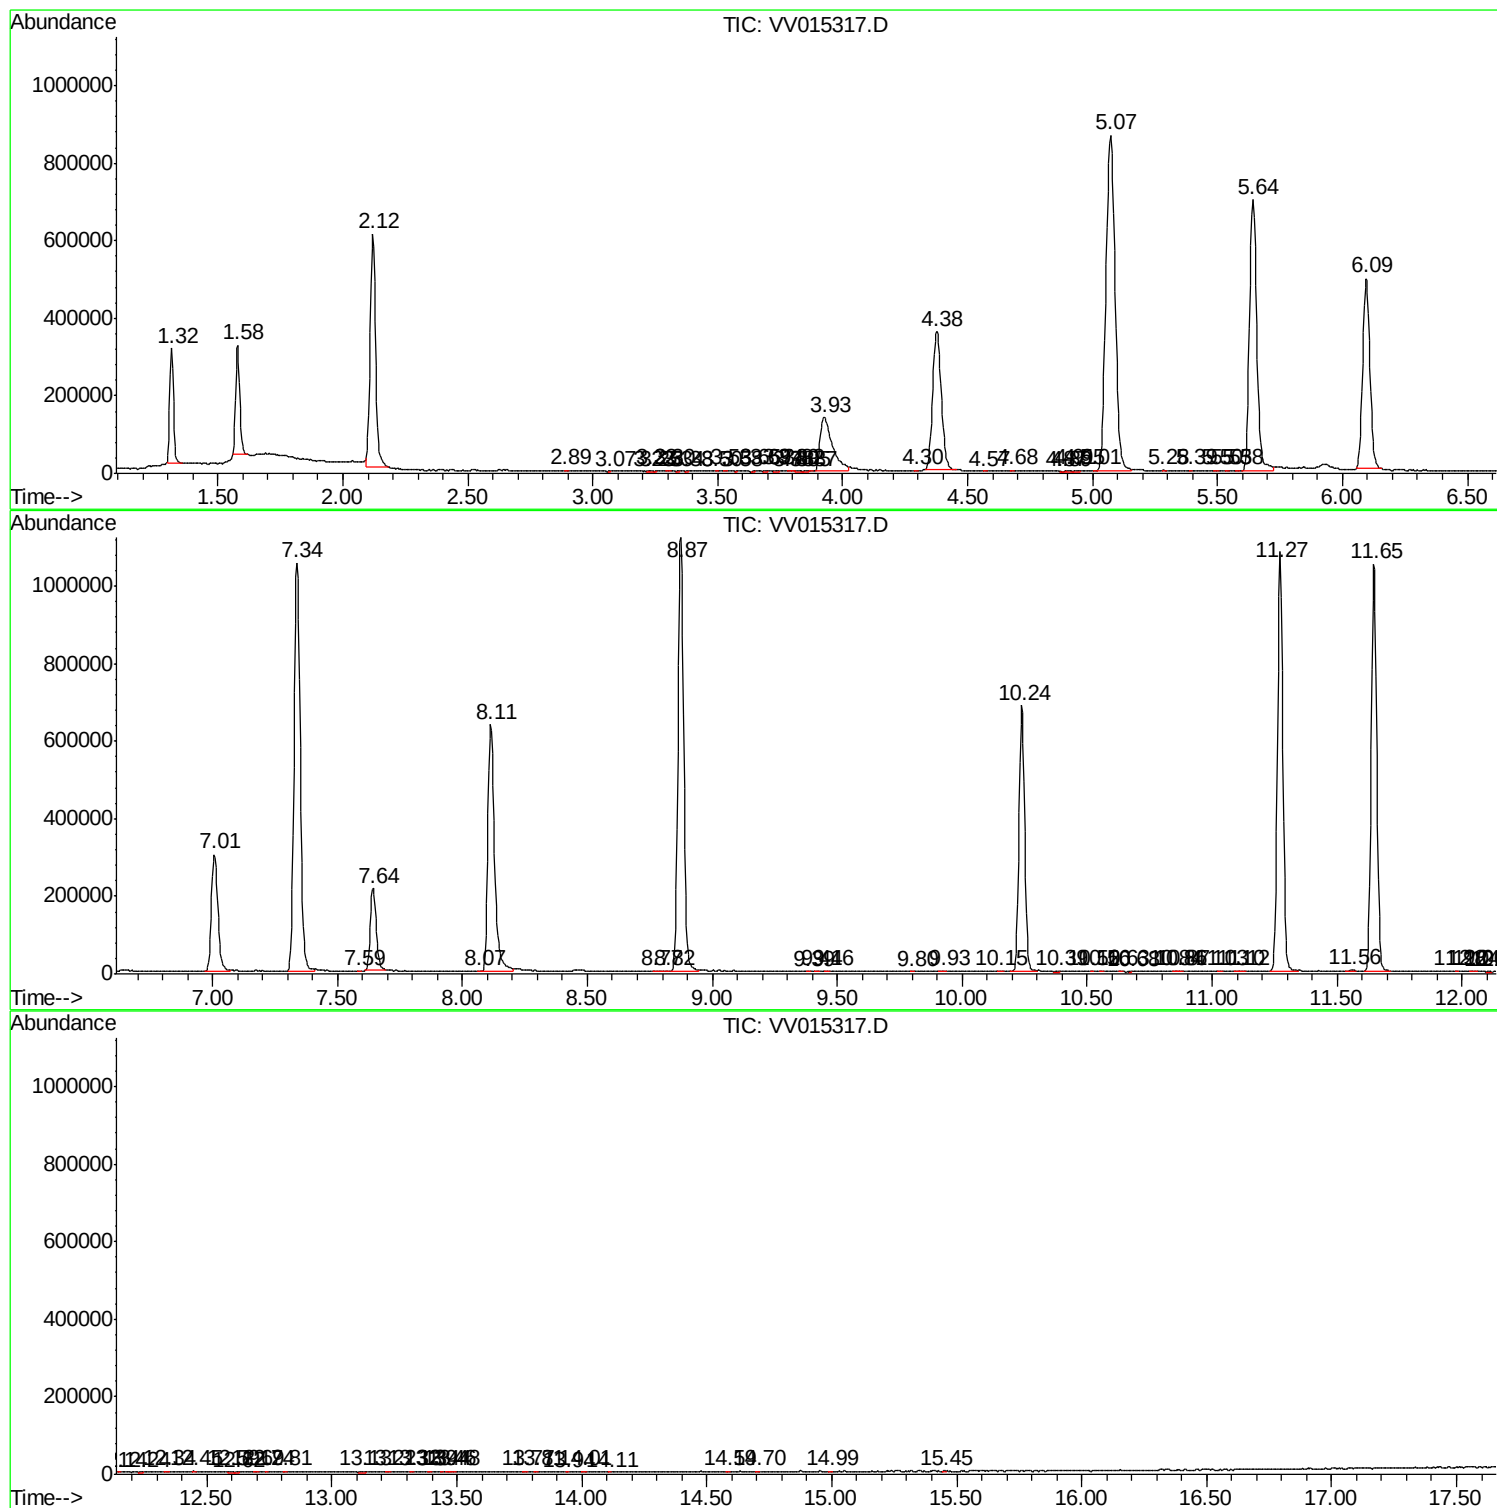

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015317.D
Acq On : 31 Mar 2020 16:36
Operator : SY/MD
Sample : VIBLK88
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK88

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015317.D
Acq On : 31 Mar 2020 16:36
Operator : SY/MD
Sample : VIBLK88
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK88

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc