

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015319.D
 Acq On : 31 Mar 2020 17:25
 Operator : SY/MD
 Sample : VIBLK89
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	84	rVB	295768	293200	13.76%	1.699%
2	1.576	146	151	171	rVB	382879	472330	22.17%	2.737%
3	2.123	313	321	338	rVB	548820	817028	38.35%	4.734%
4	2.679	491	494	495	rBV3	1394	589	0.03%	0.003%
5	2.885	555	558	561	rBV4	1643	961	0.05%	0.006%
6	3.026	601	602	604	rBV2	1115	574	0.03%	0.003%
7	3.113	623	629	633	rBV7	2370	2751	0.13%	0.016%
8	3.161	642	644	645	rBV2	1234	538	0.03%	0.003%
9	3.280	679	681	685	rBV5	1940	1509	0.07%	0.009%
10	3.370	707	709	711	rBV3	1330	681	0.03%	0.004%
11	3.418	720	724	725	rBV4	908	601	0.03%	0.003%
12	3.428	725	727	728	rBV2	1751	696	0.03%	0.004%
13	3.467	737	739	742	rVB4	1387	592	0.03%	0.003%
14	3.515	747	754	756	rBV7	1725	1847	0.09%	0.011%
15	3.566	764	770	773	rBV8	2308	1957	0.09%	0.011%
16	3.618	784	786	789	rVB3	1534	775	0.04%	0.004%
17	3.640	791	793	797	rVB4	1190	715	0.03%	0.004%
18	3.663	797	800	801	rBV3	950	391	0.02%	0.002%
19	3.692	805	809	811	rVB5	1426	770	0.04%	0.004%
20	3.705	811	813	814	rBV2	1402	637	0.03%	0.004%
21	3.756	825	829	832	rBV5	2200	1735	0.08%	0.010%
22	3.788	835	839	842	rBV6	1625	1617	0.08%	0.009%
23	3.823	848	850	853	rBV4	1452	1204	0.06%	0.007%
24	3.836	853	854	857	rVB3	1489	481	0.02%	0.003%
25	3.852	857	859	863	rVB2	1197	718	0.03%	0.004%
26	3.910	866	877	911	rBV	169208	512467	24.06%	2.969%
27	4.377	1007	1022	1045	rBV2	354774	847716	39.80%	4.912%
28	4.608	1093	1094	1097	rVB3	1295	480	0.02%	0.003%
29	4.624	1097	1099	1104	rBV6	1858	1367	0.06%	0.008%
30	4.692	1117	1120	1122	rBV3	1375	1026	0.05%	0.006%
31	4.823	1158	1161	1165	rBV5	1782	1505	0.07%	0.009%
32	4.849	1167	1169	1171	rVB3	1309	572	0.03%	0.003%
33	4.862	1171	1173	1174	rBV2	918	324	0.02%	0.002%
34	4.885	1178	1180	1184	rBV4	1374	1040	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015319.D
 Acq On : 31 Mar 2020 17:25
 Operator : SY/MD
 Sample : VIBLK89
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	4.904	1184	1186	1188	rVB3	1356	637	0.03%	0.004%
36	4.923	1190	1192	1194	rBV3	1771	733	0.03%	0.004%
37	4.971	1205	1207	1211	rVB4	2211	1404	0.07%	0.008%
38	4.994	1211	1214	1216	rBV3	1521	821	0.04%	0.005%
39	5.071	1221	1238	1265	rBV2	835358	2130191	100.00%	12.343%
40	5.245	1289	1292	1297	rBV7	1817	1793	0.08%	0.010%
41	5.476	1362	1364	1365	rBV2	1463	534	0.03%	0.003%
42	5.492	1367	1369	1371	rVV3	1871	941	0.04%	0.005%
43	5.592	1390	1400	1401	rBV	20661	30502	1.43%	0.177%
44	5.640	1405	1415	1438	rVB	658883	1329896	62.43%	7.706%
45	6.093	1545	1556	1583	rVB	500752	1007287	47.29%	5.836%
46	6.601	1710	1714	1716	rBV4	2792	2430	0.11%	0.014%
47	6.788	1770	1772	1775	rBV3	1753	990	0.05%	0.006%
48	7.007	1826	1840	1855	rBV	299371	532949	25.02%	3.088%
49	7.338	1931	1943	1964	rBV	1033024	1774898	83.32%	10.284%
50	7.643	2028	2038	2053	rVB2	207350	344896	16.19%	1.998%
51	8.109	2173	2183	2209	rBV	681858	1192861	56.00%	6.912%
52	8.875	2410	2421	2441	rVB	1038561	1653050	77.60%	9.578%
53	9.537	2625	2627	2628	rBV2	1194	591	0.03%	0.003%
54	10.010	2768	2774	2776	rBV6	2736	2735	0.13%	0.016%
55	10.238	2830	2845	2861	rBV	697480	1097583	51.53%	6.360%
56	10.347	2877	2879	2881	rBV3	1781	800	0.04%	0.005%
57	10.370	2884	2886	2889	rBV4	1574	856	0.04%	0.005%
58	10.492	2920	2924	2926	rBV6	1471	982	0.05%	0.006%
59	10.630	2964	2967	2968	rBV3	974	651	0.03%	0.004%
60	10.817	3023	3025	3029	rBV5	1547	950	0.04%	0.006%
61	11.151	3127	3129	3132	rBV3	1693	772	0.04%	0.004%
62	11.270	3154	3166	3183	rBV	1018282	1551611	72.84%	8.990%
63	11.524	3243	3245	3249	rBV4	2265	1926	0.09%	0.011%
64	11.646	3272	3283	3303	rBV	1030003	1586423	74.47%	9.192%
65	11.900	3360	3362	3365	rBV3	1194	745	0.03%	0.004%
66	12.048	3406	3408	3411	rBV4	1696	1187	0.06%	0.007%
67	12.222	3459	3462	3465	rBV4	2141	1362	0.06%	0.008%
68	12.283	3479	3481	3482	rBV2	1333	516	0.02%	0.003%
69	12.322	3490	3493	3497	rBV5	2187	1747	0.08%	0.010%
70	12.357	3501	3504	3505	rBV3	1743	986	0.05%	0.006%
71	12.482	3541	3543	3546	rBV3	1924	1424	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015319.D
Acq On : 31 Mar 2020 17:25
Operator : SY/MD
Sample : VIBLK89
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK89

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Title : VOC Analysis

72	12.511	3550	3552	3557	rVB6	1591	1404	0.07%	0.008%
73	12.537	3558	3560	3561	rBV2	979	370	0.02%	0.002%
74	12.592	3569	3577	3578	rBV6	2439	2789	0.13%	0.016%
75	12.695	3606	3609	3613	rBV6	2660	2190	0.10%	0.013%
76	12.717	3613	3616	3619	rBV3	1461	966	0.05%	0.006%
77	12.733	3619	3621	3623	rVB3	1007	371	0.02%	0.002%
78	12.749	3623	3626	3628	rBV3	1162	862	0.04%	0.005%
79	12.804	3639	3643	3644	rBV4	1956	1324	0.06%	0.008%
80	12.961	3687	3692	3697	rBV9	2410	3161	0.15%	0.018%
81	13.067	3722	3725	3726	rBV3	1378	766	0.04%	0.004%
82	13.077	3726	3728	3731	rVV4	1441	696	0.03%	0.004%
83	13.823	3954	3960	3962	rBV7	2259	2105	0.10%	0.012%
84	13.945	3995	3998	4001	rBV4	2262	1233	0.06%	0.007%
85	14.067	4033	4036	4040	rBV4	1435	1373	0.06%	0.008%
86	14.241	4086	4090	4094	rBV6	2461	2264	0.11%	0.013%
87	14.283	4101	4103	4107	rBV5	1316	1007	0.05%	0.006%
88	14.431	4146	4149	4151	rBV3	2063	1054	0.05%	0.006%
89	14.453	4151	4156	4157	rBV4	3131	2544	0.12%	0.015%
90	14.550	4184	4186	4187	rBV2	1213	392	0.02%	0.002%


Sum of corrected areas: 17258925

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015319.D
Acq On : 31 Mar 2020 17:25
Operator : SY/MD
Sample : VIBLK89
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK89

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

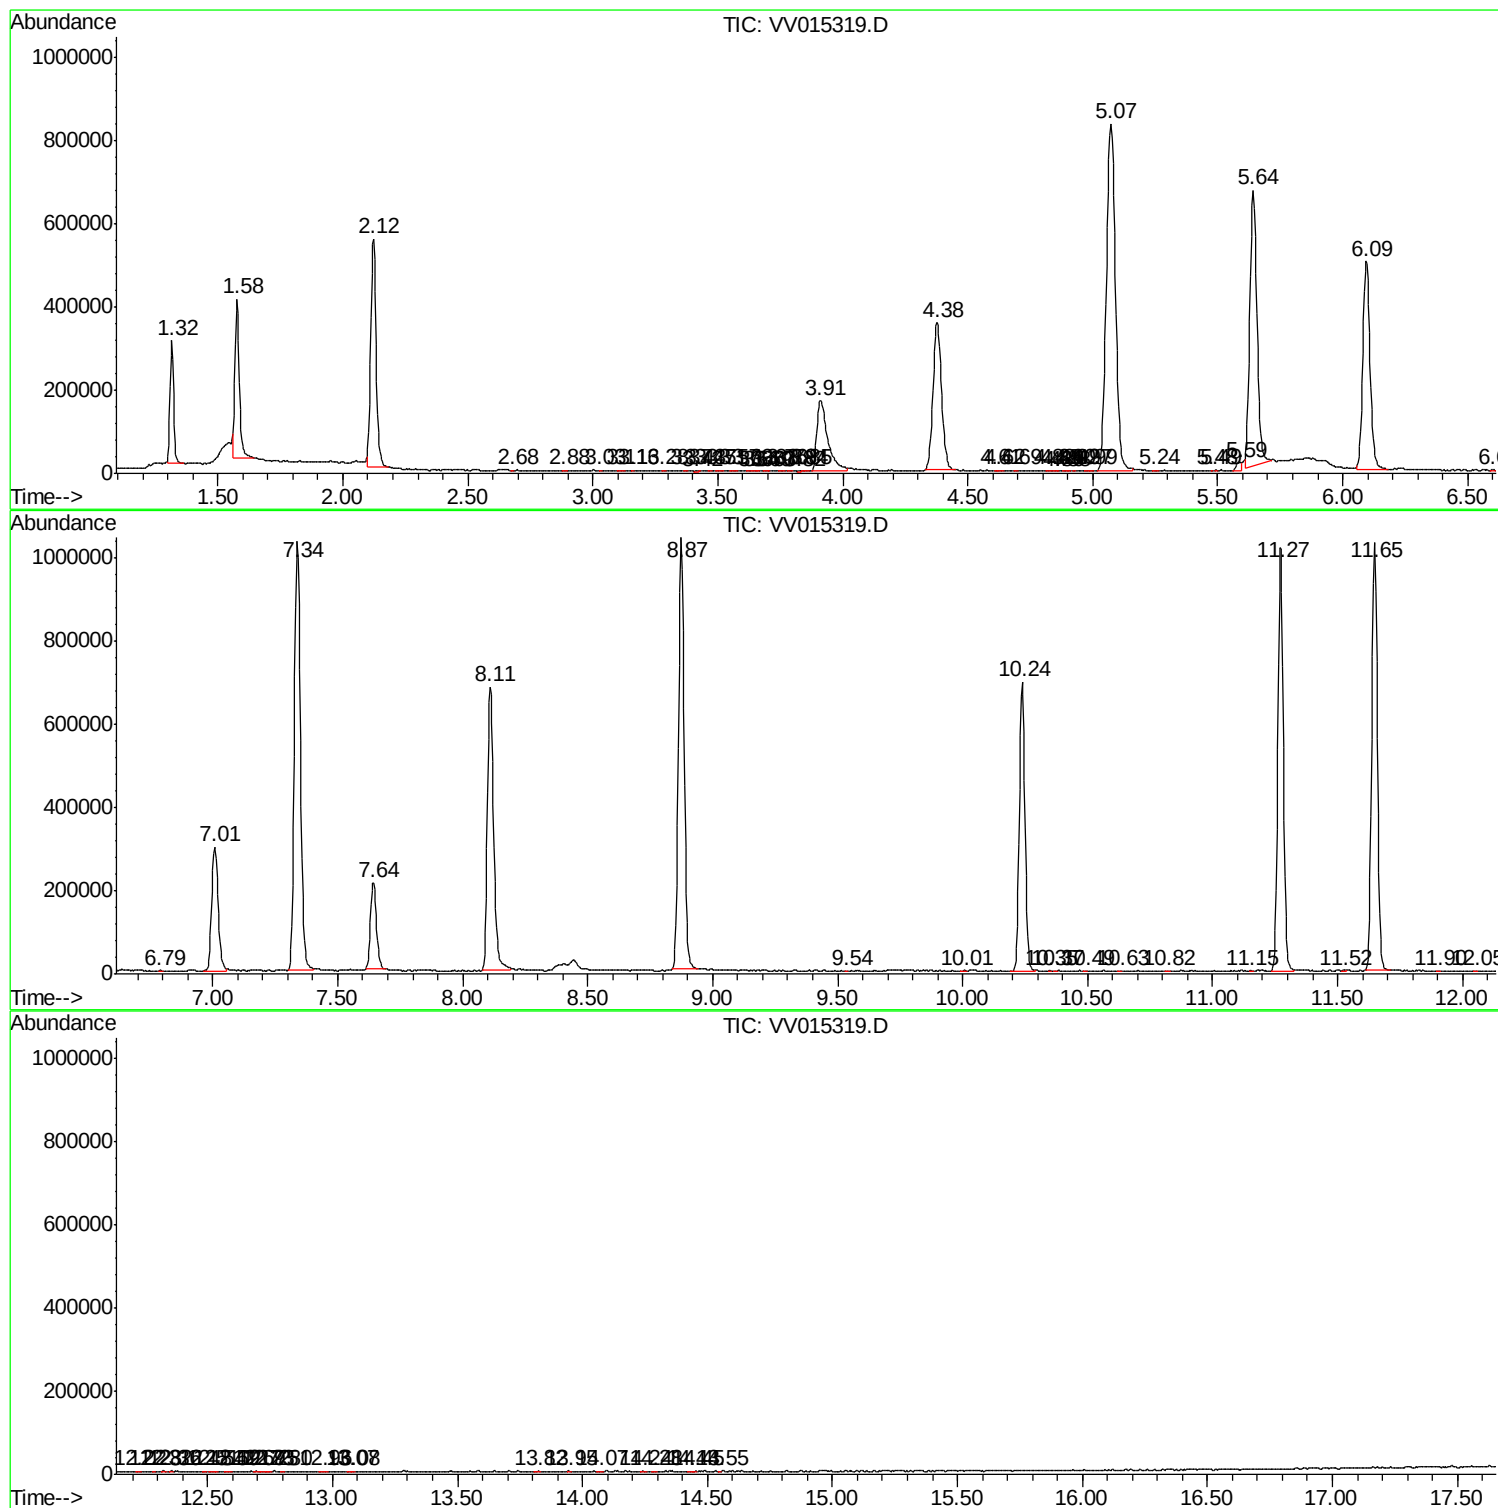

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015319.D
Acq On : 31 Mar 2020 17:25
Operator : SY/MD
Sample : VIBLK89
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK89

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV033120\
Data File : VV015319.D
Acq On : 31 Mar 2020 17:25
Operator : SY/MD
Sample : VIBLK89
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK89

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc