

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015320.D
 Acq On : 31 Mar 2020 17:49
 Operator : SY/MD
 Sample : L1975-15 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	85	rVB2	746193	804344	26.87%	3.895%
2	1.579	146	152	165	rBV	354660	412596	13.78%	1.998%
3	2.122	313	321	342	rVB	564962	850925	28.43%	4.120%
4	2.727	507	509	513	rVB4	1413	731	0.02%	0.004%
5	2.984	586	589	591	rBV4	1604	1101	0.04%	0.005%
6	3.016	597	599	601	rBV2	1286	817	0.03%	0.004%
7	3.058	609	612	614	rBV3	1425	967	0.03%	0.005%
8	3.145	634	639	640	rBV5	1432	1134	0.04%	0.005%
9	3.367	706	708	709	rBV2	1072	389	0.01%	0.002%
10	3.383	709	713	716	rVV5	2843	2265	0.08%	0.011%
11	3.550	762	765	766	rBV3	1239	687	0.02%	0.003%
12	3.637	790	792	795	rVB3	1267	704	0.02%	0.003%
13	3.656	795	798	799	rBV3	1278	747	0.02%	0.004%
14	3.727	818	820	821	rBV2	1138	484	0.02%	0.002%
15	3.833	852	853	854	rBV	939	269	0.01%	0.001%
16	3.939	866	886	917	rBV2	1131718	2993433	100.00%	14.495%
17	4.376	1009	1022	1045	rVB	350909	846299	28.27%	4.098%
18	4.659	1107	1110	1113	rBV5	2231	1593	0.05%	0.008%
19	4.746	1136	1137	1138	rBV	1403	454	0.02%	0.002%
20	4.785	1148	1149	1151	rVB2	1163	393	0.01%	0.002%
21	4.801	1152	1154	1155	rBV2	1611	541	0.02%	0.003%
22	4.839	1164	1166	1169	rBV4	1289	914	0.03%	0.004%
23	4.900	1182	1185	1189	rBV6	2135	2120	0.07%	0.010%
24	5.074	1220	1239	1267	rBV2	847197	2163795	72.28%	10.478%
25	5.325	1315	1317	1318	rBV2	1542	642	0.02%	0.003%
26	5.437	1350	1352	1354	rBV3	1527	909	0.03%	0.004%
27	5.489	1364	1368	1369	rBV4	2221	1365	0.05%	0.007%
28	5.643	1403	1416	1438	rBV	710617	1457508	48.69%	7.058%
29	6.093	1544	1556	1582	rVB	504929	1005076	33.58%	4.867%
30	6.331	1625	1630	1633	rBV7	2886	3225	0.11%	0.016%
31	6.617	1717	1719	1720	rBV2	1686	592	0.02%	0.003%
32	6.826	1782	1784	1789	rVB5	2221	1851	0.06%	0.009%
33	6.852	1789	1792	1793	rBV3	1643	1011	0.03%	0.005%
34	6.926	1812	1815	1818	rBV5	1719	990	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015320.D
 Acq On : 31 Mar 2020 17:49
 Operator : SY/MD
 Sample : L1975-15 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	6.949	1818	1822	1823	rBV4	1724	1033	0.03%	0.005%
36	7.006	1830	1840	1857	rBV	302239	529959	17.70%	2.566%
37	7.338	1929	1943	1962	rBV	1055387	1827488	61.05%	8.849%
38	7.643	2028	2038	2054	rBV	212176	356758	11.92%	1.728%
39	7.968	2136	2139	2144	rBV7	2275	1962	0.07%	0.010%
40	8.113	2173	2184	2209	rBV	678512	1218128	40.69%	5.899%
41	8.875	2410	2421	2440	rBV	1096908	1768609	59.08%	8.564%
42	9.958	2755	2758	2761	rBV4	1764	988	0.03%	0.005%
43	10.238	2833	2845	2861	rBV	699834	1096156	36.62%	5.308%
44	10.440	2906	2908	2911	rBV4	1716	1213	0.04%	0.006%
45	10.511	2927	2930	2934	rBV4	2112	2159	0.07%	0.010%
46	10.685	2982	2984	2986	rBV3	1027	526	0.02%	0.003%
47	10.752	3000	3005	3006	rBV4	1219	773	0.03%	0.004%
48	10.846	3032	3034	3035	rBV2	896	333	0.01%	0.002%
49	10.868	3038	3041	3043	rBV4	2002	1396	0.05%	0.007%
50	10.919	3055	3057	3060	rBV4	1097	856	0.03%	0.004%
51	11.029	3089	3091	3096	rVB5	1660	1285	0.04%	0.006%
52	11.273	3155	3167	3182	rBV	1067931	1630170	54.46%	7.894%
53	11.649	3271	3284	3305	rBV	1030685	1607171	53.69%	7.782%
54	11.849	3342	3346	3349	rBV5	2297	2100	0.07%	0.010%
55	11.923	3367	3369	3374	rBV6	1673	1261	0.04%	0.006%
56	12.029	3400	3402	3404	rBV3	1369	722	0.02%	0.003%
57	12.157	3440	3442	3445	rBV3	1729	1218	0.04%	0.006%
58	12.427	3522	3526	3528	rBV5	1189	870	0.03%	0.004%
59	12.546	3561	3563	3564	rBV2	1419	501	0.02%	0.002%
60	12.907	3672	3675	3679	rBV5	1646	1119	0.04%	0.005%
61	12.939	3683	3685	3686	rBV2	1220	499	0.02%	0.002%
62	13.035	3712	3715	3717	rVB4	1975	1048	0.04%	0.005%
63	13.138	3745	3747	3749	rBV3	1213	593	0.02%	0.003%
64	13.289	3783	3794	3797	rBV10	2834	4950	0.17%	0.024%
65	13.373	3817	3820	3823	rBV5	2273	1848	0.06%	0.009%
66	13.405	3826	3830	3835	rVB	34026	19757	0.66%	0.096%
67	13.653	3905	3907	3909	rBV2	1000	555	0.02%	0.003%
68	13.662	3909	3910	3913	rVV3	1487	705	0.02%	0.003%
69	13.762	3937	3941	3944	rBV6	2930	2964	0.10%	0.014%
70	13.939	3993	3996	3999	rBV4	2433	1442	0.05%	0.007%
71	14.196	4075	4076	4078	rBV2	1177	460	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015320.D
Acq On : 31 Mar 2020 17:49
Operator : SY/MD
Sample : L1975-15 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Title : VOC Analysis

72	14.820	4268	4270	4272	rBV3	1644	841	0.03%	0.004%
----	--------	------	------	------	------	------	-----	-------	--------


Sum of corrected areas: 20651287

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015320.D
Acq On : 31 Mar 2020 17:49
Operator : SY/MD
Sample : L1975-15 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

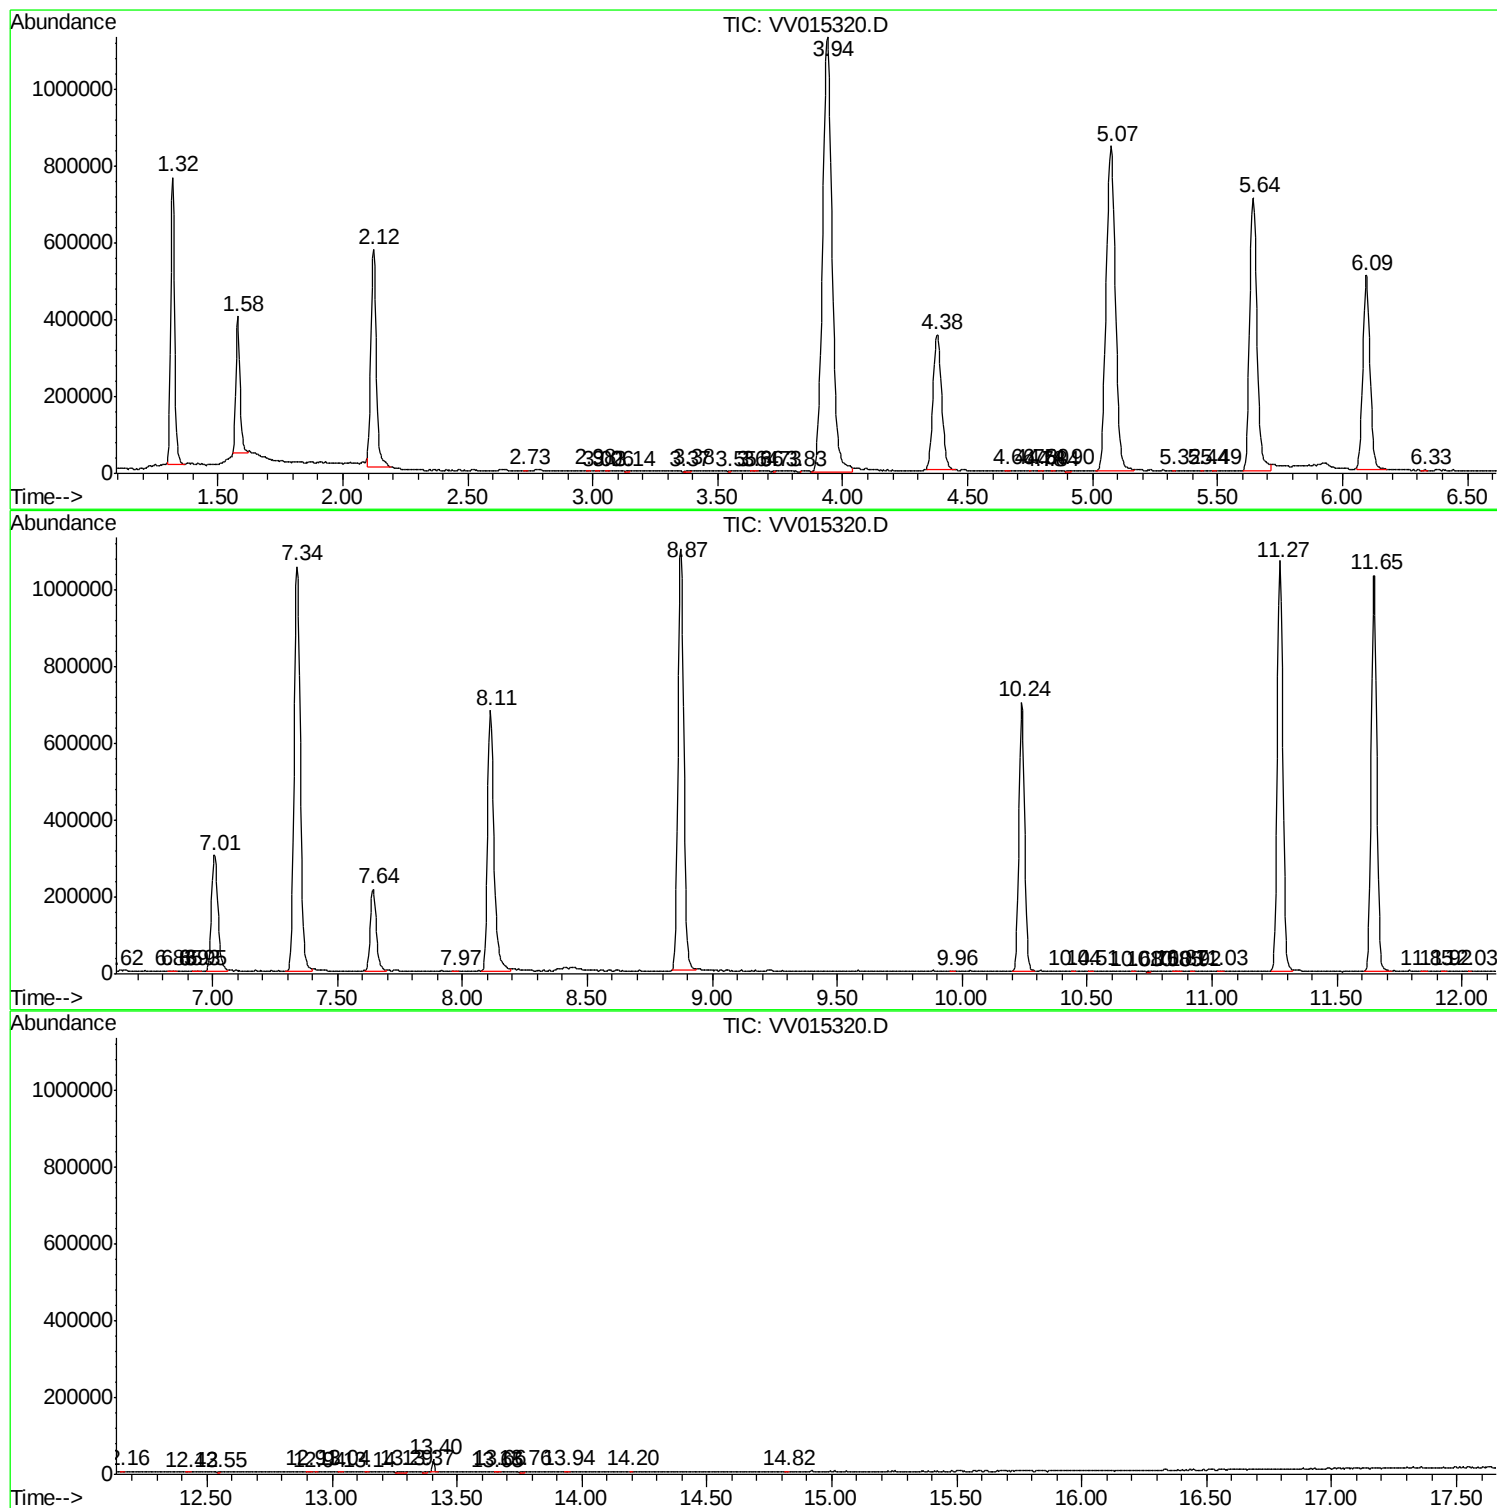

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015320.D
Acq On : 31 Mar 2020 17:49
Operator : SY/MD
Sample : L1975-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015320.D
Acq On : 31 Mar 2020 17:49
Operator : SY/MD
Sample : L1975-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc