

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015321.D
 Acq On : 31 Mar 2020 18:13
 Operator : SY/MD
 Sample : L1975-08 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	88	rVB2	1543220	1631645	49.67%	7.374%
2	1.579	146	152	164	rBV	304250	364663	11.10%	1.648%
3	2.122	313	321	342	rVB	565581	863410	26.29%	3.902%
4	2.920	567	569	573	rVB4	1353	797	0.02%	0.004%
5	2.949	575	578	580	rBV4	944	657	0.02%	0.003%
6	2.962	580	582	584	rBV3	1340	788	0.02%	0.004%
7	3.048	606	609	611	rBV3	1214	998	0.03%	0.005%
8	3.077	615	618	620	rBV4	1182	688	0.02%	0.003%
9	3.138	634	637	640	rBV4	2541	1858	0.06%	0.008%
10	3.235	666	667	668	rBV	851	287	0.01%	0.001%
11	3.254	668	673	678	rVB8	2855	2845	0.09%	0.013%
12	3.273	678	679	681	rBV2	1037	457	0.01%	0.002%
13	3.302	685	688	691	rVB5	1563	830	0.03%	0.004%
14	3.376	709	711	713	rVB3	2129	847	0.03%	0.004%
15	3.441	728	731	735	rVB4	1853	1245	0.04%	0.006%
16	3.460	735	737	738	rBV2	1176	381	0.01%	0.002%
17	3.598	778	780	782	rVB3	1677	764	0.02%	0.003%
18	3.614	782	785	786	rBV3	733	304	0.01%	0.001%
19	3.679	801	805	807	rBV5	1194	668	0.02%	0.003%
20	3.695	807	810	814	rVV5	1730	1304	0.04%	0.006%
21	3.756	824	829	831	rBV6	1658	1691	0.05%	0.008%
22	3.814	845	847	848	rBV2	758	249	0.01%	0.001%
23	3.833	849	853	854	rBV4	2967	1838	0.06%	0.008%
24	3.939	869	886	922	rBV2	1246645	3284733	100.00%	14.845%
25	4.376	1008	1022	1048	rVB	354837	859191	26.16%	3.883%
26	4.695	1115	1121	1122	rBV5	2093	1982	0.06%	0.009%
27	4.759	1136	1141	1143	rBV6	1693	1367	0.04%	0.006%
28	4.833	1162	1164	1165	rBV2	2006	831	0.03%	0.004%
29	4.878	1176	1178	1179	rBV2	1422	683	0.02%	0.003%
30	4.904	1184	1186	1190	rVV4	1228	961	0.03%	0.004%
31	4.926	1191	1193	1197	rVB4	1598	887	0.03%	0.004%
32	4.978	1207	1209	1210	rBV2	1565	524	0.02%	0.002%
33	5.074	1221	1239	1270	rBV2	842336	2148424	65.41%	9.710%
34	5.447	1352	1355	1356	rBV3	1201	697	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
 Data File : VV015321.D
 Acq On : 31 Mar 2020 18:13
 Operator : SY/MD
 Sample : L1975-08 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis

35	5.460	1356	1359	1361	rVV4	1624	1140	0.03%	0.005%
36	5.643	1402	1416	1434	rBV	705958	1414211	43.05%	6.392%
37	6.096	1545	1557	1580	rVB	492332	990459	30.15%	4.476%
38	6.852	1788	1792	1795	rBV5	2898	2177	0.07%	0.010%
39	6.871	1795	1798	1800	rVV3	1237	630	0.02%	0.003%
40	7.006	1829	1840	1855	rBV	299196	527600	16.06%	2.384%
41	7.338	1931	1943	1963	rBV	1043412	1797456	54.72%	8.124%
42	7.588	2018	2021	2023	rBV3	2186	1251	0.04%	0.006%
43	7.643	2027	2038	2057	rVV	215410	368799	11.23%	1.667%
44	7.984	2140	2144	2146	rBV5	2338	1824	0.06%	0.008%
45	8.112	2172	2184	2213	rBV	744380	1373556	41.82%	6.208%
46	8.733	2369	2377	2393	rVB2	32212	52868	1.61%	0.239%
47	8.874	2409	2421	2442	rBV	1124043	1802419	54.87%	8.146%
48	9.653	2659	2663	2668	rBV8	2182	2338	0.07%	0.011%
49	9.730	2680	2687	2700	rBV2	34068	54757	1.67%	0.247%
50	10.112	2803	2806	2810	rBV5	2395	2243	0.07%	0.010%
51	10.193	2828	2831	2833	rBV4	1362	844	0.03%	0.004%
52	10.238	2834	2845	2860	rVV	734010	1127746	34.33%	5.097%
53	10.508	2927	2929	2931	rBV3	1128	467	0.01%	0.002%
54	10.768	3008	3010	3011	rBV2	1025	215	0.01%	0.001%
55	11.067	3096	3103	3117	rVB2	25415	42099	1.28%	0.190%
56	11.270	3155	3166	3186	rBV	1121343	1698593	51.71%	7.677%
57	11.646	3272	3283	3301	rBV	1084351	1651259	50.27%	7.463%
58	11.833	3338	3341	3342	rBV3	1608	985	0.03%	0.004%
59	12.103	3424	3425	3427	rBV2	1423	743	0.02%	0.003%
60	12.196	3452	3454	3456	rBV3	1227	529	0.02%	0.002%
61	12.222	3460	3462	3465	rBV3	1690	1012	0.03%	0.005%
62	12.334	3494	3497	3502	rBV7	2441	2527	0.08%	0.011%
63	12.424	3521	3525	3529	rBV6	1773	2062	0.06%	0.009%
64	12.517	3549	3554	3557	rBV7	2472	2529	0.08%	0.011%
65	12.550	3560	3564	3565	rBV3	1292	872	0.03%	0.004%
66	12.607	3579	3582	3587	rBV6	1205	1084	0.03%	0.005%
67	12.977	3695	3697	3700	rVB3	1209	574	0.02%	0.003%
68	13.061	3719	3723	3725	rBV2	2008	1585	0.05%	0.007%
69	13.196	3761	3765	3767	rBV5	2101	1288	0.04%	0.006%
70	13.495	3855	3858	3863	rVB6	1872	1332	0.04%	0.006%
71	13.646	3900	3905	3910	rBV7	2180	2097	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015321.D
Acq On : 31 Mar 2020 18:13
Operator : SY/MD
Sample : L1975-08 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Title : VOC Analysis

72	13.987	4009	4011	4013	rBV3	1400	512	0.02%	0.002%
73	14.003	4013	4016	4021	rVB6	3598	3167	0.10%	0.014%
74	14.029	4021	4024	4025	rBV3	2097	1323	0.04%	0.006%
75	14.099	4044	4046	4049	rBV3	1413	550	0.02%	0.002%
76	14.173	4067	4069	4071	rBV3	1986	968	0.03%	0.004%
77	14.302	4107	4109	4110	rBV2	1081	382	0.01%	0.002%
78	14.373	4129	4131	4135	rBV3	1747	1052	0.03%	0.005%
79	14.572	4191	4193	4196	rBV4	1257	624	0.02%	0.003%
80	14.617	4205	4207	4209	rBV2	2318	966	0.03%	0.004%
81	14.649	4215	4217	4219	rBV2	1438	763	0.02%	0.003%
82	14.662	4219	4221	4223	rVB3	1751	721	0.02%	0.003%
83	15.019	4329	4332	4334	rBV3	2319	1566	0.05%	0.007%


Sum of corrected areas: 22126258

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV033120\
Data File : VV015321.D
Acq On : 31 Mar 2020 18:13
Operator : SY/MD
Sample : L1975-08 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

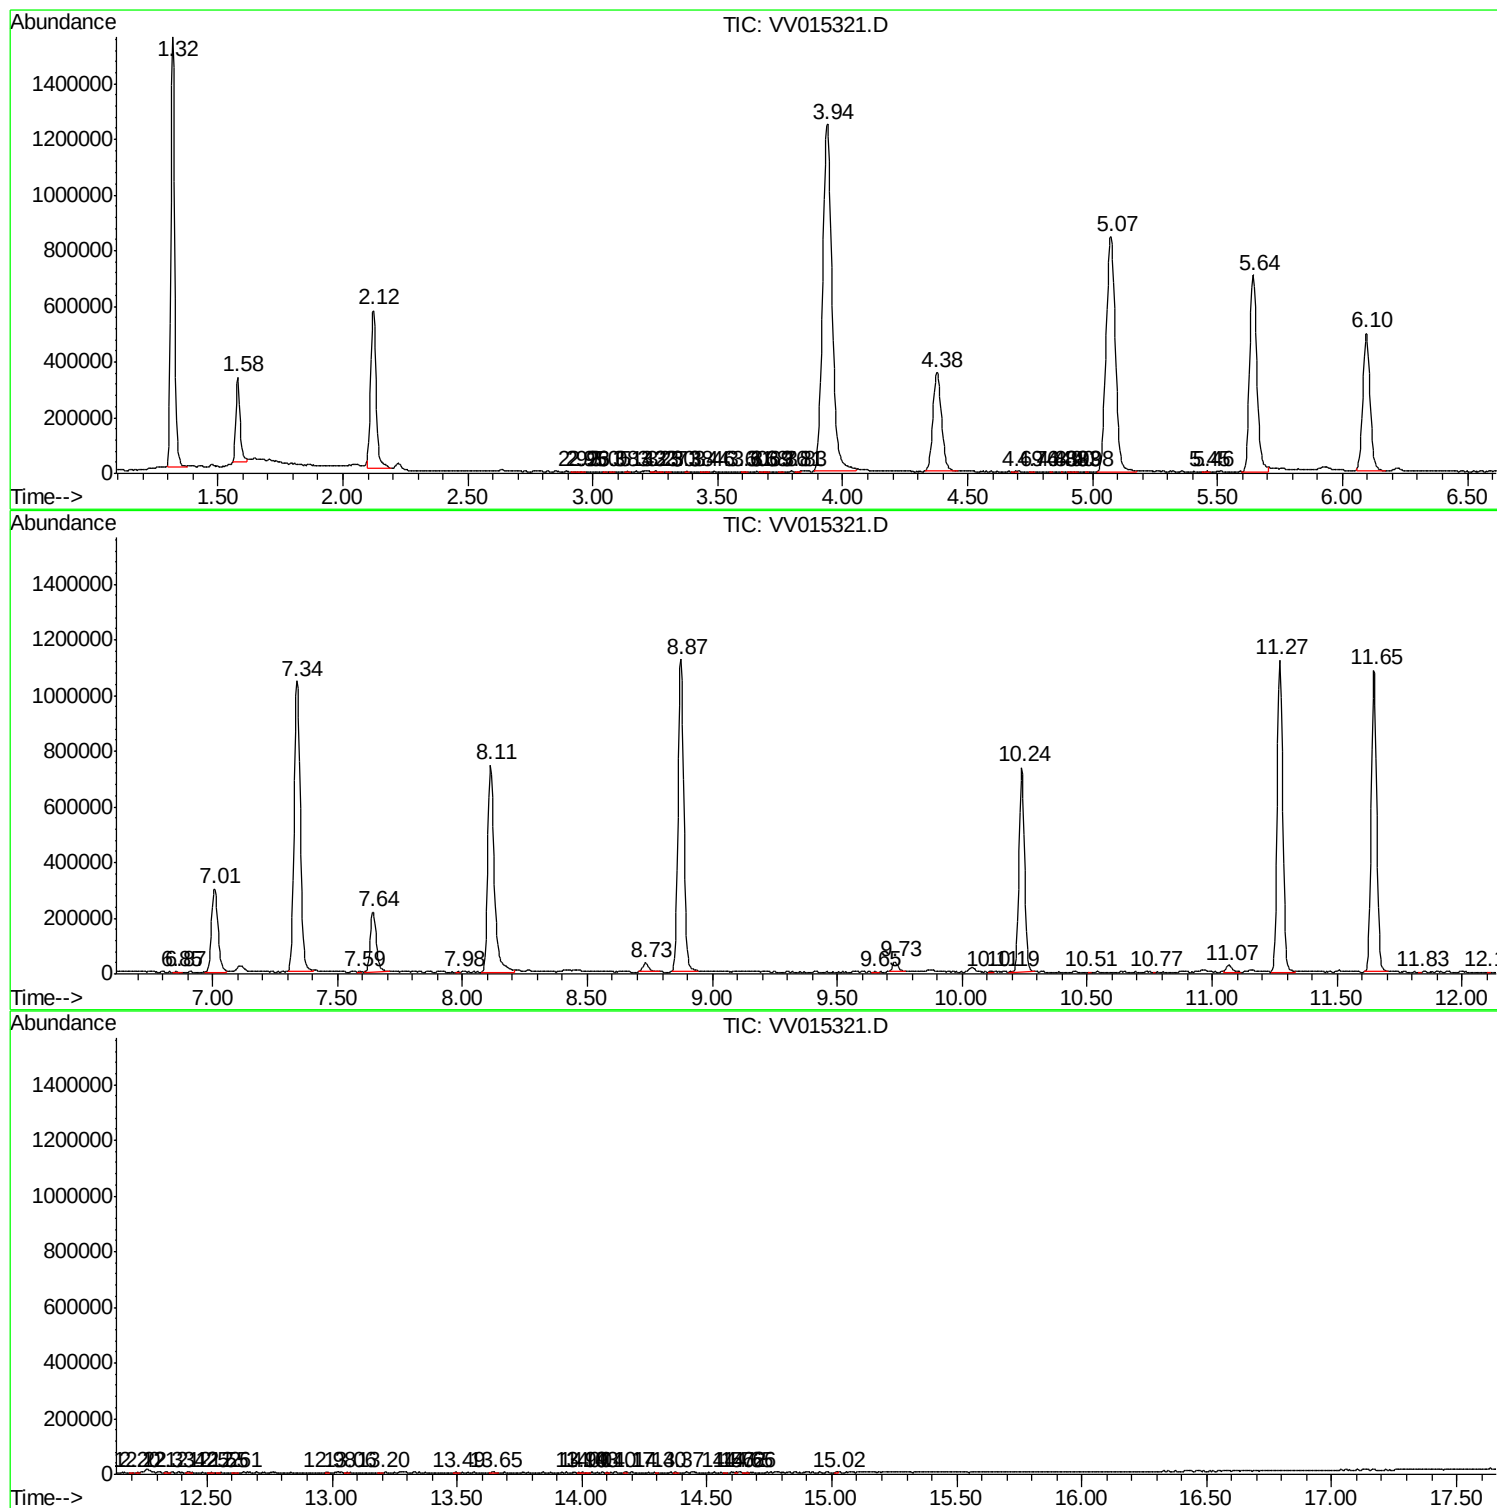

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015321.D
Acq On : 31 Mar 2020 18:13
Operator : SY/MD
Sample : L1975-08 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033120\
Data File : VV015321.D
Acq On : 31 Mar 2020 18:13
Operator : SY/MD
Sample : L1975-08 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
